

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat No :RP10795
 Lot No :E1075520J
 Time Processed :7:18:58 AM
 Month-Day-Year Processed :11/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

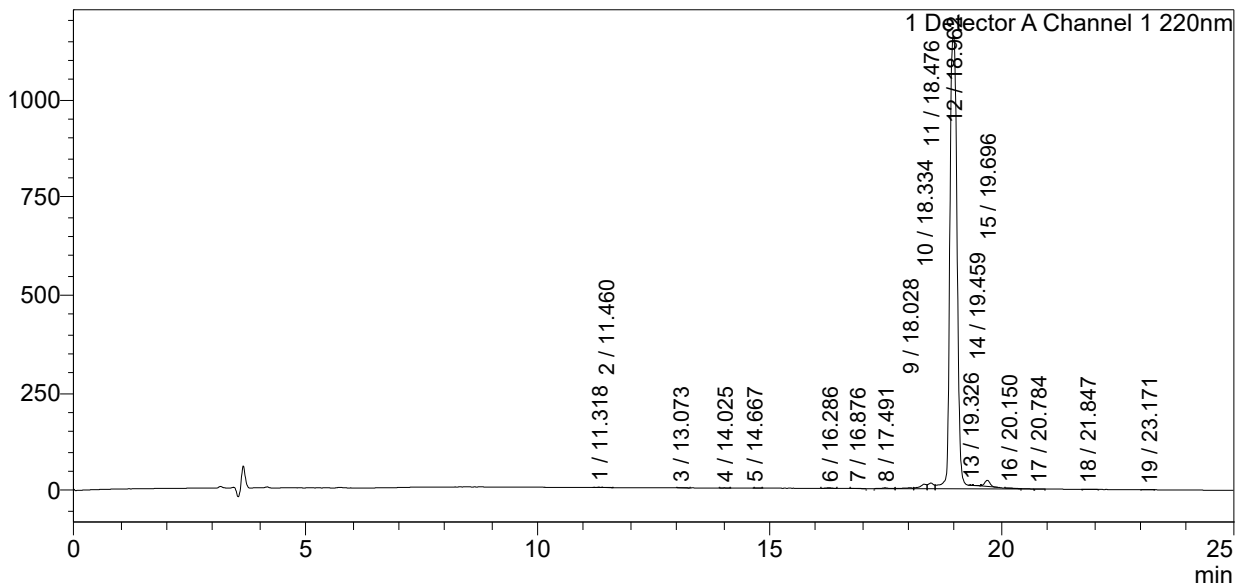

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.318	5343	820	0.040
2	11.460	4745	644	0.036
3	13.073	1900	178	0.014
4	14.025	2899	404	0.022
5	14.667	1130	145	0.009
6	16.286	14768	1677	0.112
7	16.876	5258	691	0.040
8	17.491	22729	2145	0.172
9	18.028	33228	2280	0.251
10	18.334	116516	11575	0.881
11	18.476	130227	14553	0.985
12	18.962	12738835	1158421	96.324
13	19.326	1877	443	0.014
14	19.459	5407	879	0.041
15	19.696	126910	15872	0.960
16	20.150	5571	595	0.042

Peak#	Ret. Time	Area	Height	Area%
17	20.784	1306	203	0.010
18	21.847	3912	382	0.030
19	23.171	2397	309	0.018
Total		13224955	1212216	100.000