

Sample Name: mTRP-2(180-188)
 Cat No. : RP20250
 Lot No. : E4773319J
 Time Processed: 8:58:44 AM
 Month-Day-Year Processed :10/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

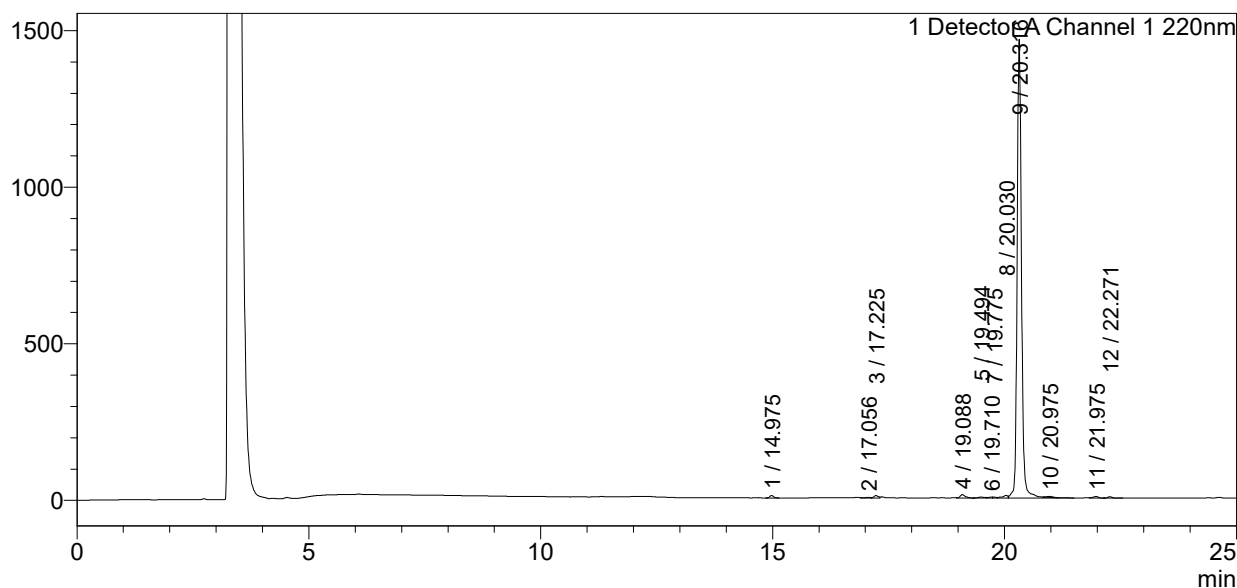

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.975	42066	7792	0.417
2	17.056	19874	2141	0.197
3	17.225	51236	7810	0.508
4	19.088	81349	10868	0.807
5	19.494	29407	3013	0.292
6	19.710	16325	2584	0.162
7	19.775	14676	2625	0.146
8	20.030	66912	8165	0.664
9	20.316	9655962	1464906	95.811
10	20.975	26230	2663	0.260
11	21.975	43561	5371	0.432
12	22.271	30556	4574	0.303
Total		10078155	1522513	100.000