


Mass Spectrum

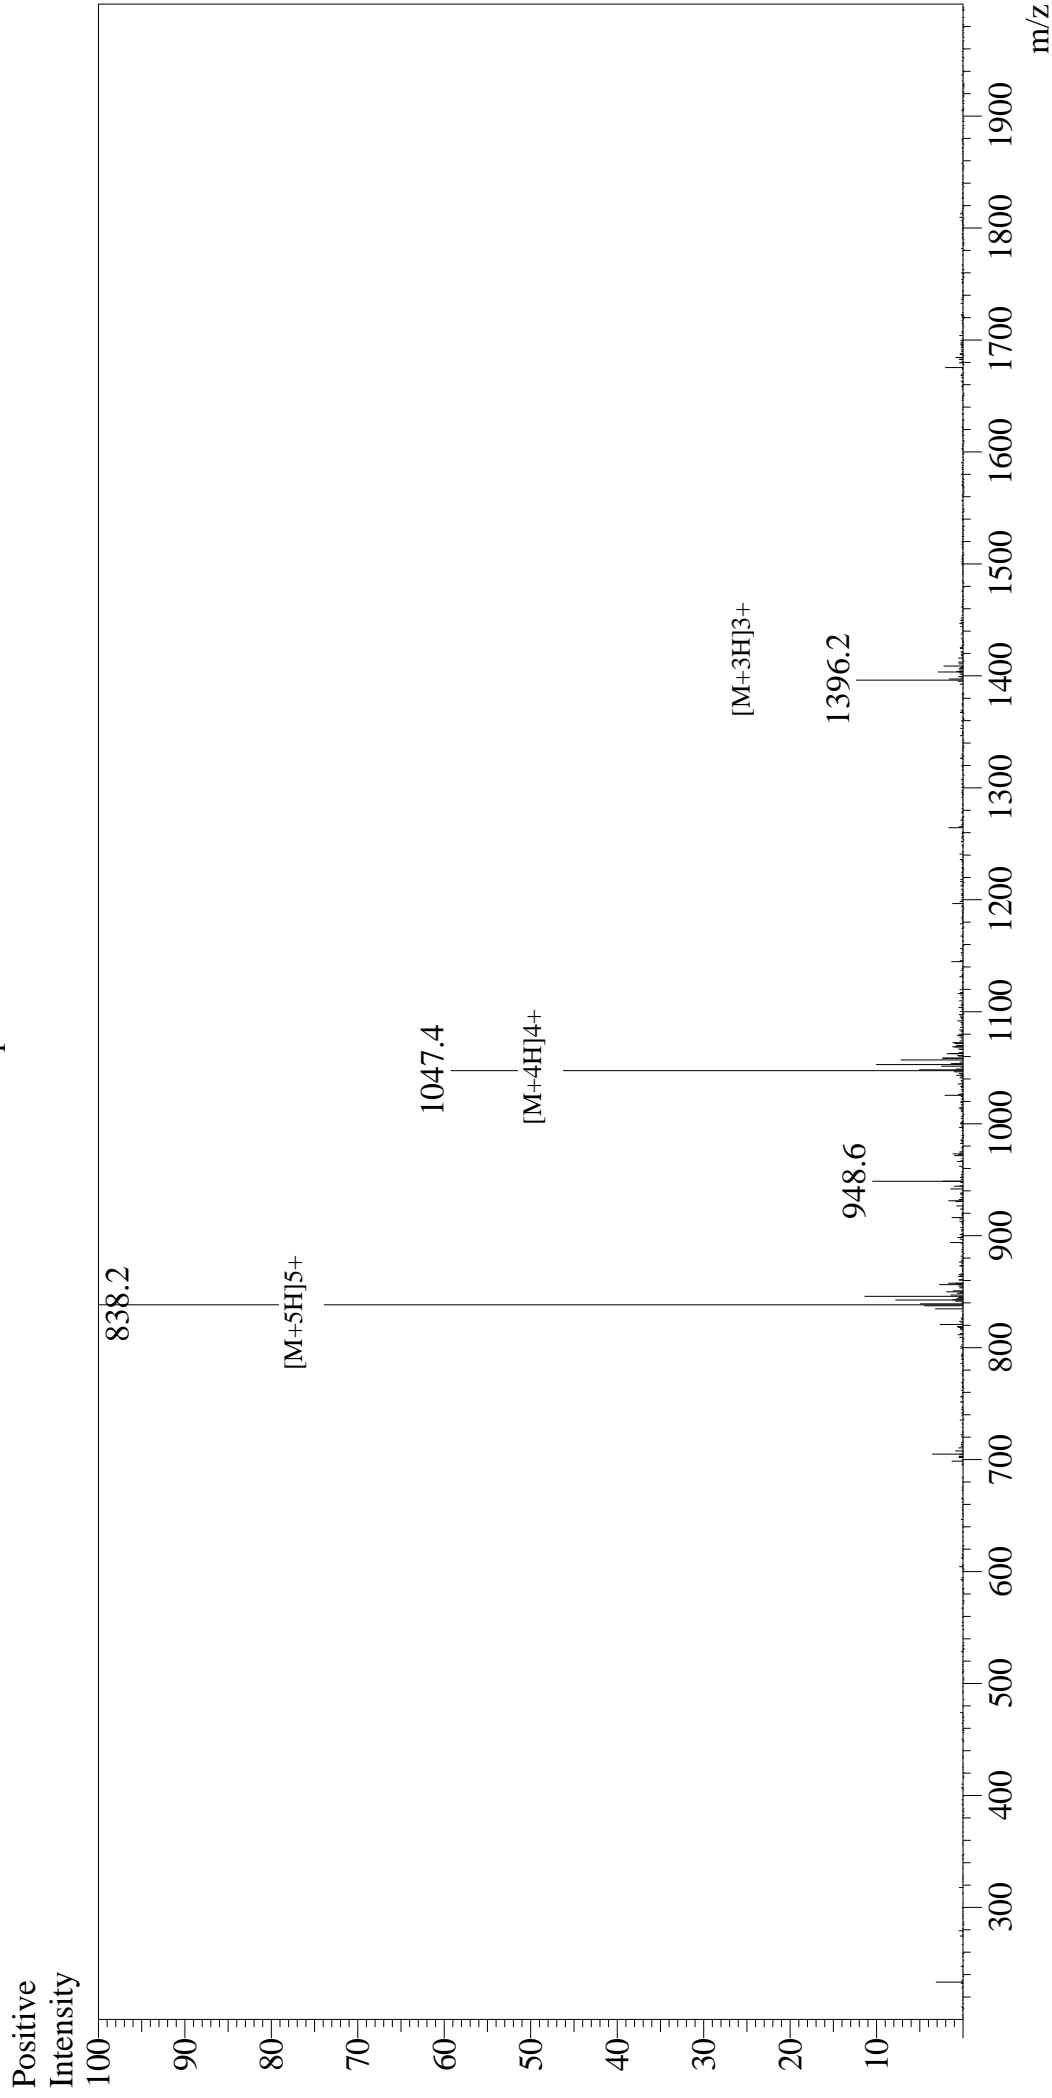

Sample Information

User : Gary
Month-Day Processed : 03/18/19
Time Processed : 15:28:38
Injection Volume : 0.2
Sample Name : Exendin-4
Cat No. : RP10874
Lot No. : PE0221903
Theoretical MW : 4186.66
Observed MW : 4186.0

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH