

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No. : RP11095
 Lot No. : E4730120K
 Time Processed : 12:34:04 PM
 Month-Day-Year Processed : 11/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
95.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

mV

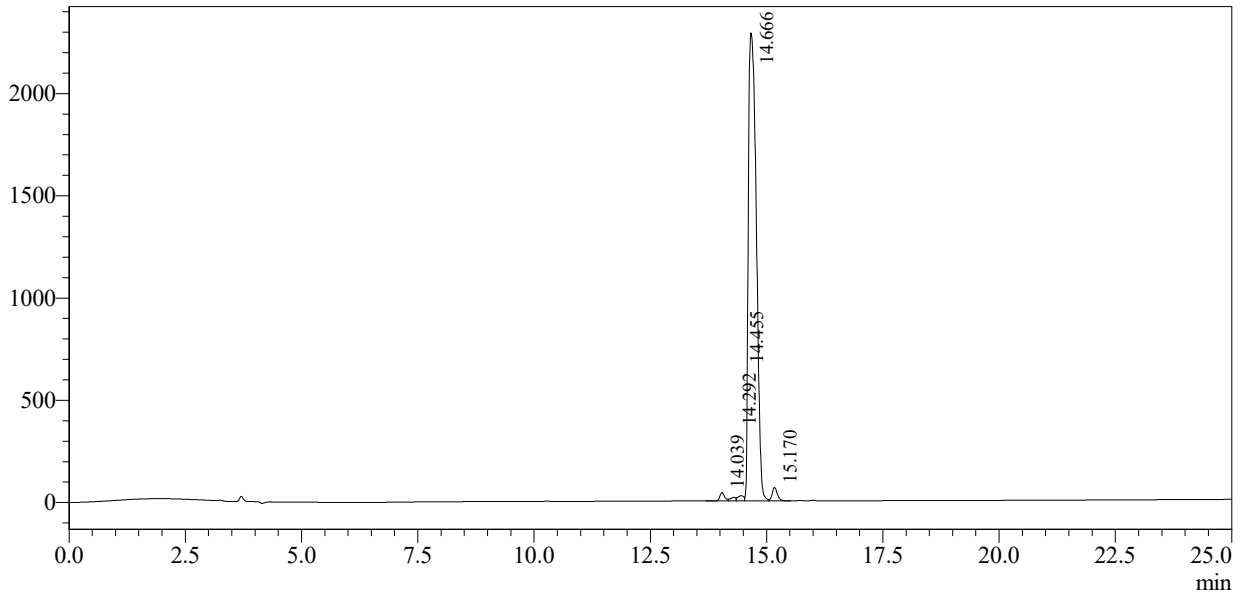

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.039	291862	40685	1.027
2	14.292	141960	17433	0.499
3	14.455	221219	25577	0.778
4	14.666	27266579	2288597	95.926
5	15.170	502952	65152	1.769
Total		28424572	2437445	100.000