

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat  
 Cat No. : RP11095  
 Lot No. : E8359521F  
 Time Processed : 17:05:31  
 Month-Day-Year Processed : 07/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK12010012

<Chromatogram>

mV

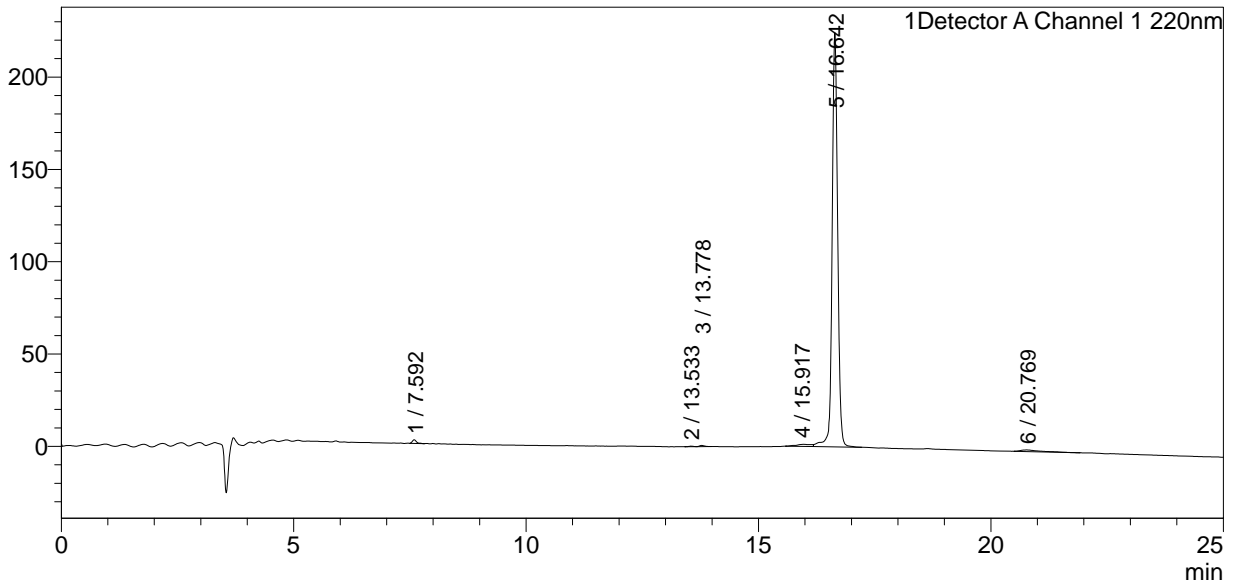

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.592	12046	1922	0.626
2	13.533	1908	243	0.099
3	13.778	4592	630	0.239
4	15.917	26430	1065	1.374
5	16.642	1852379	222949	96.288
6	20.769	26433	869	1.374
Total		1923788	227679	100.000