

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat No. :RP11110
 Lot No. :E7158920G
 Time Processed :16:21:38
 Month-Day-Year Processed :07/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

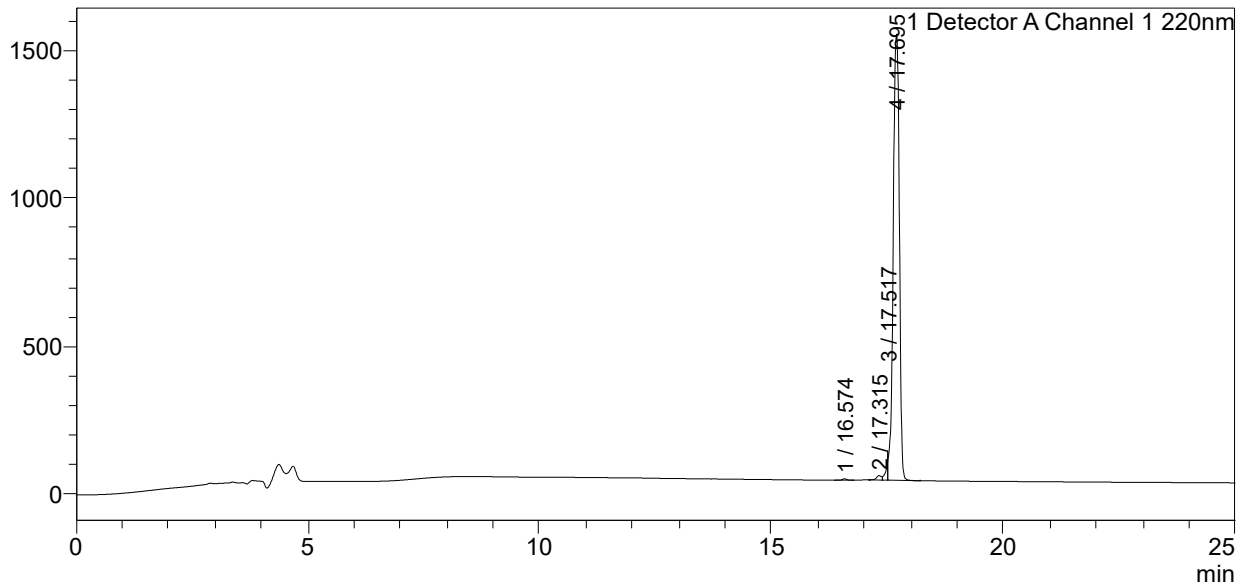

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.574	29481	4591	0.208
2	17.315	112220	15058	0.792
3	17.517	335852	67805	2.371
4	17.695	13688904	1503967	96.629
Total		14166457	1591421	100.000