

Sample Name :PAR-4 Agonist Peptide, amide  
 Cat No. :RP11529  
 Lot No. :E0768721F  
 Time Processed :2:10:42 AM  
 Month-Day-Year Processed :06/30/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

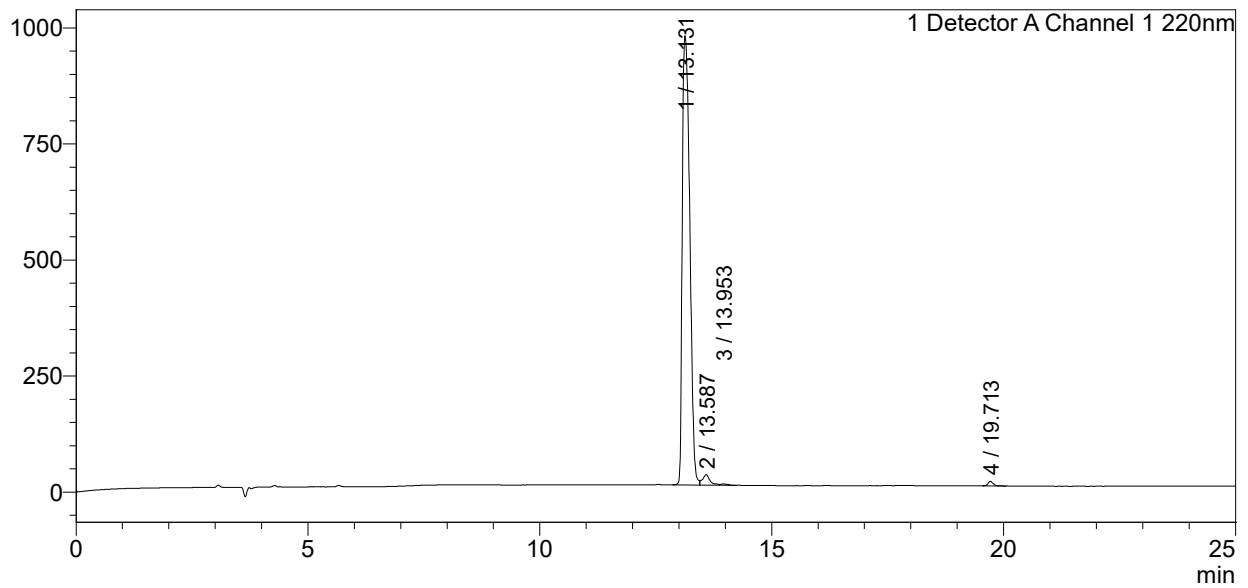

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.131	10804345	968102	96.838
2	13.587	248778	22234	2.230
3	13.953	29519	2655	0.265
4	19.713	74511	9951	0.668
Total		11157154	1002942	100.000