

Sample Name : β -Amyloid (25-35)
 Cat No. :RP10008
 Lot No. :E1589720G
 Time Processed :7:29:46
 Month-Day-Year Processed :08/08/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 35.00 | Pumps | Solvent B Conc. | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

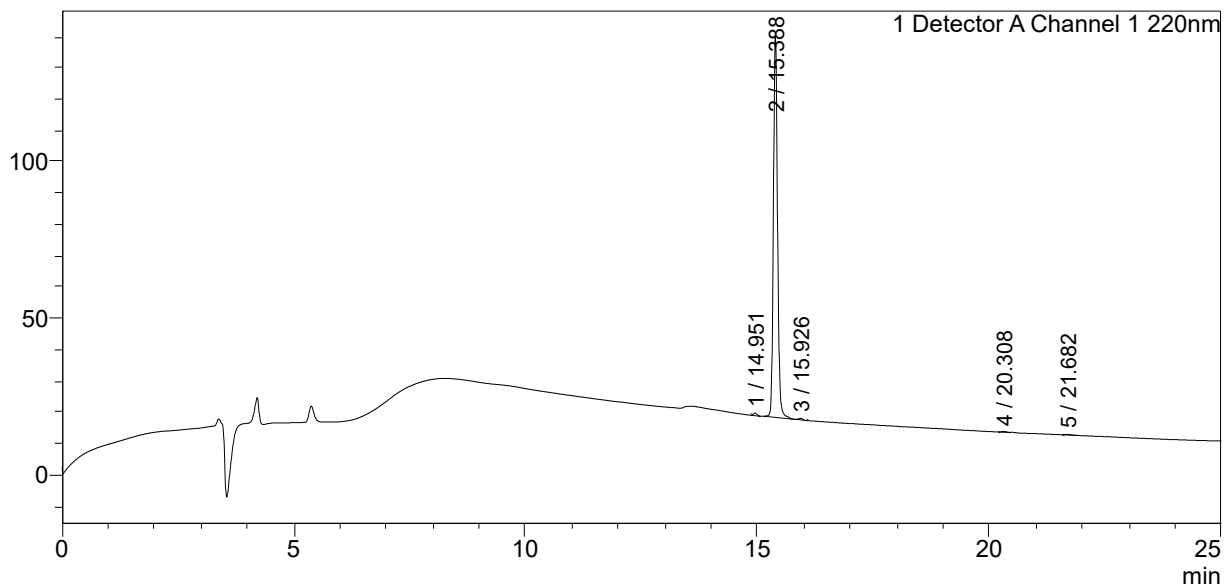

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|--------|--------|---------|
| 1 | 14.951 | 4333 | 832 | 0.566 |
| 2 | 15.388 | 755580 | 121695 | 98.661 |
| 3 | 15.926 | 2718 | 491 | 0.355 |
| 4 | 20.308 | 1551 | 196 | 0.202 |
| 5 | 21.682 | 1652 | 168 | 0.216 |
| Total | | 765834 | 123381 | 100.000 |