

Sample Name :Cortistatin 14,human,rat
 Cat No. :RP10972
 Lot No. :PE7261904
 Time Processed :8:38:25
 Month-Day-Year Processed :04/17/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

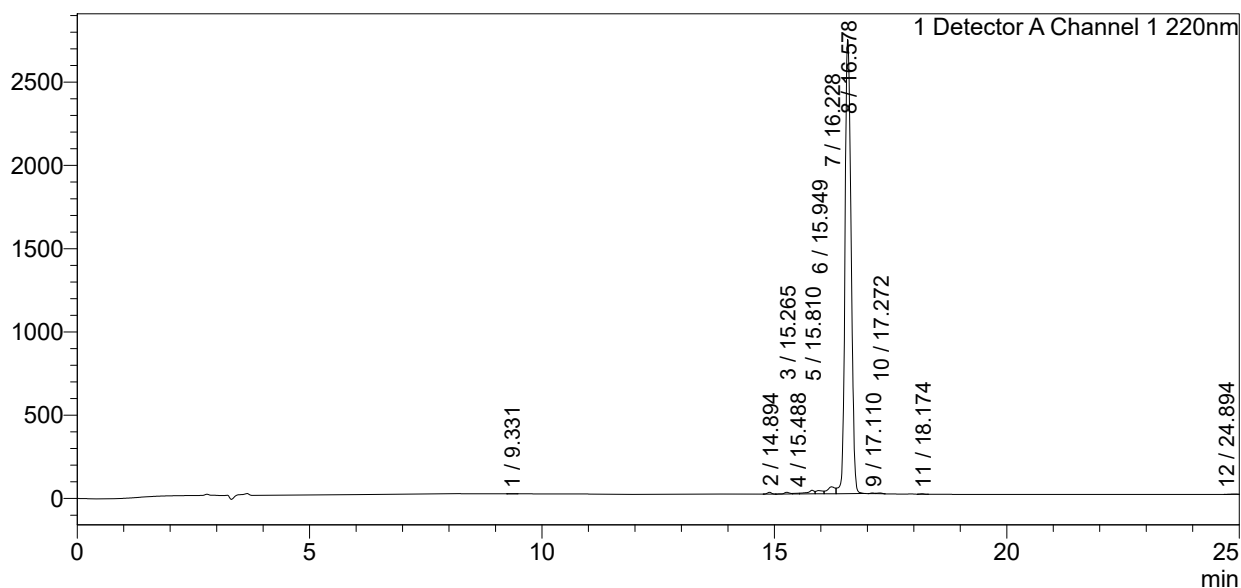

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.331	2035	346	0.008
2	14.894	63058	10897	0.243
3	15.265	80614	10265	0.311
4	15.488	36940	5005	0.142
5	15.810	218486	21522	0.842
6	15.949	200347	19533	0.772
7	16.228	478543	41561	1.844
8	16.578	24783282	2727419	95.495
9	17.110	25647	3946	0.099
10	17.272	34117	4952	0.131
11	18.174	16151	2949	0.062
12	24.894	13250	1406	0.051
Total		25952469	2849801	100.000