

Sample Name :HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE4301902
 Time Processed : 10:27:28
 Month-Day-Year Processed : 02/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

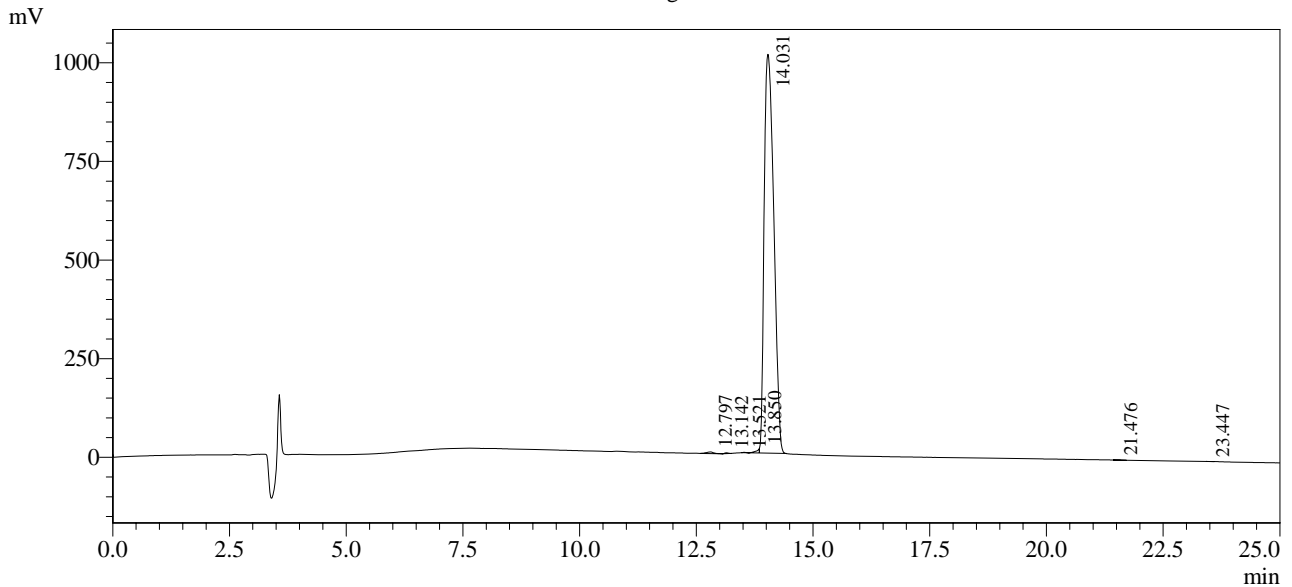

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.797	42029	4078	0.288
2	13.142	9819	1928	0.067
3	13.521	4471	972	0.031
4	13.850	49209	11285	0.338
5	14.031	14468821	1011249	99.257
6	21.476	1418	128	0.010
7	23.447	1369	225	0.009
Total		14577136	1029865	100.000