

Sample Name: Rabies Virus Glycoprotein

Cat. No. : RP20464 Lot. No. : PE0191805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

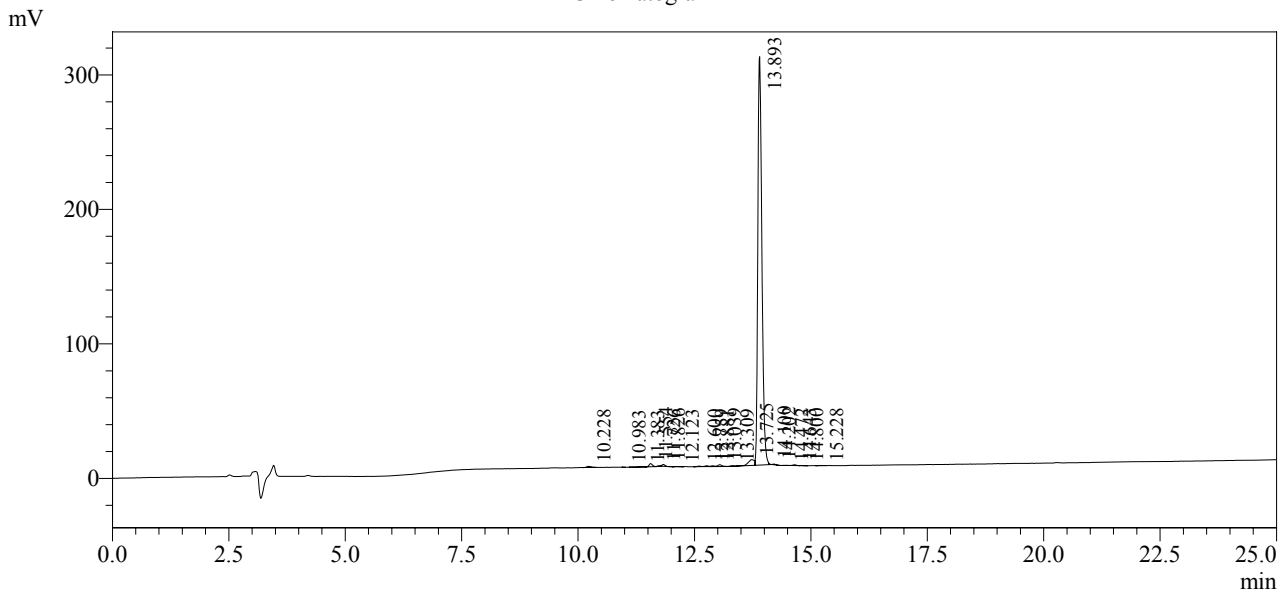

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.228	4792	798	0.248
2	10.983	11	10	0.001
3	11.383	923	71	0.048
4	11.554	11450	2333	0.593
5	11.726	785	259	0.041
6	11.826	6359	1373	0.330
7	12.123	1382	218	0.072
8	12.600	2574	401	0.133
9	12.759	3257	617	0.169
10	12.881	2923	576	0.151
11	13.039	7907	1303	0.410
12	13.309	1404	300	0.073
13	13.725	39551	4295	2.049
14	13.893	1836279	303598	95.148
15	14.100	1411	1043	0.073
16	14.202	1977	515	0.102
17	14.472	816	174	0.042
18	14.643	3310	620	0.172
19	14.800	978	204	0.051
20	15.228	1838	343	0.095
Total		1929928	319051	100.000