

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. :RP11529
 Lot No. :E289021E
 Time Processed :11:53:48 AM
 Month-Day-Year Processed :05/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

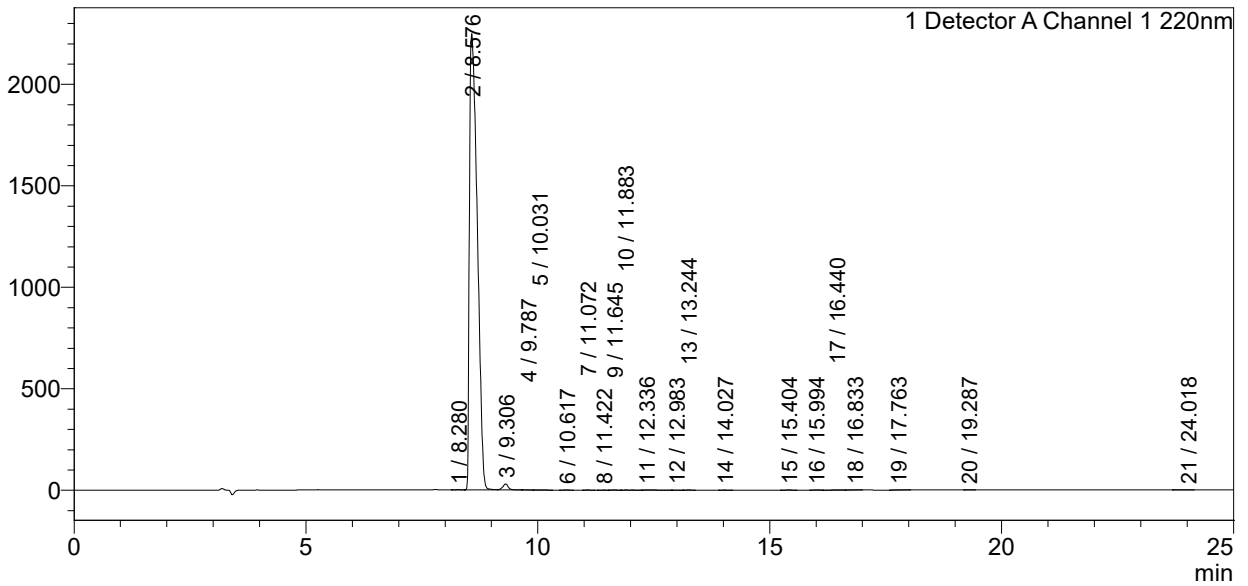

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.280	7043	1219	0.026
2	8.576	26370635	2241877	98.646
3	9.306	250344	29689	0.936
4	9.787	8618	1011	0.032
5	10.031	13359	857	0.050
6	10.617	3415	603	0.013
7	11.072	2595	444	0.010
8	11.422	3023	352	0.011
9	11.645	6008	699	0.022
10	11.883	9412	474	0.035
11	12.336	14284	571	0.053
12	12.983	1233	161	0.005
13	13.244	3437	488	0.013
14	14.027	2014	274	0.008

Peak#	Ret. Time	Area	Height	Area%
15	15.404	4456	574	0.017
16	15.994	6387	927	0.024
17	16.440	10670	1180	0.040
18	16.833	2360	236	0.009
19	17.763	6775	602	0.025
20	19.287	2247	376	0.008
21	24.018	4164	303	0.016
Total		26732478	2282918	100.000