

Sample Name :C-Peptide (3-33), human
 Cat No. :RP11116
 Lot No. :E0322820B
 Time Processed :8:56:31
 Month-Day-Year Processed :02/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

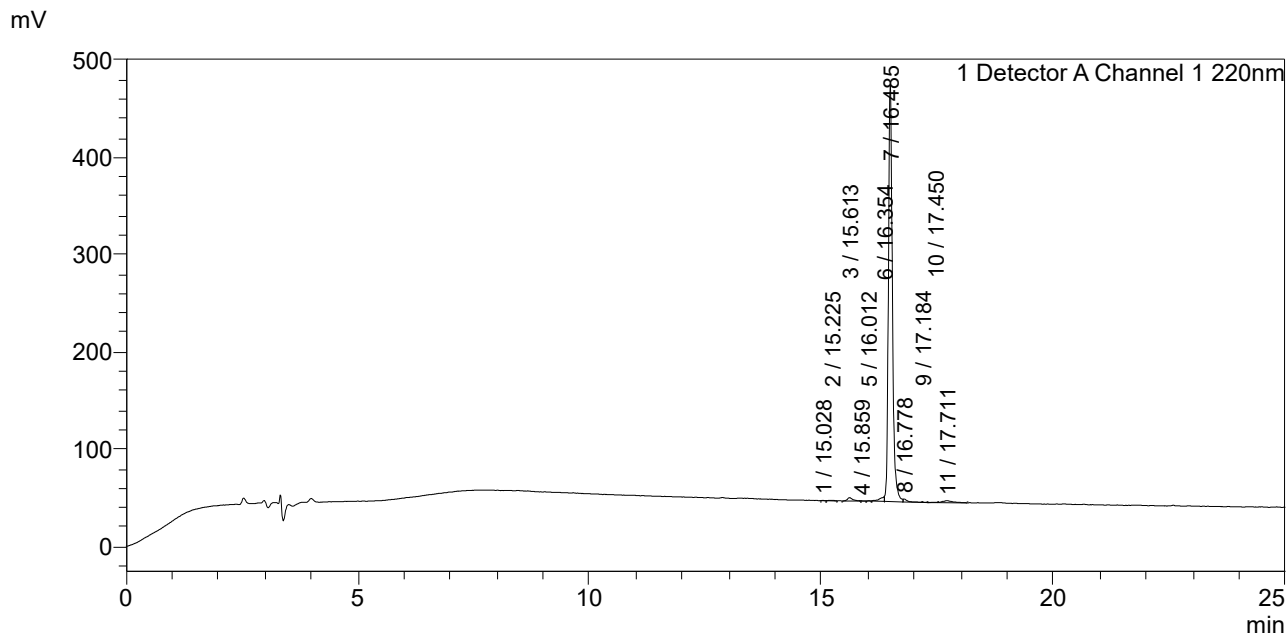

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.028	1104	307	0.041
2	15.225	4532	557	0.167
3	15.613	29732	3495	1.096
4	15.859	1596	441	0.059
5	16.012	1768	419	0.065
6	16.354	36490	4792	1.345
7	16.485	2581473	428414	95.142
8	16.778	18393	2965	0.678
9	17.184	1293	314	0.048
10	17.450	3125	393	0.115
11	17.711	33775	2217	1.245
Total		2713280	444314	100.000