

Sample Name:β-Amyloid (25-35)  
 Cat No. :RP10008  
 Lot No. :E1317521F  
 Time Processed :21:02:29  
 Month-Day-Year Processed :06/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

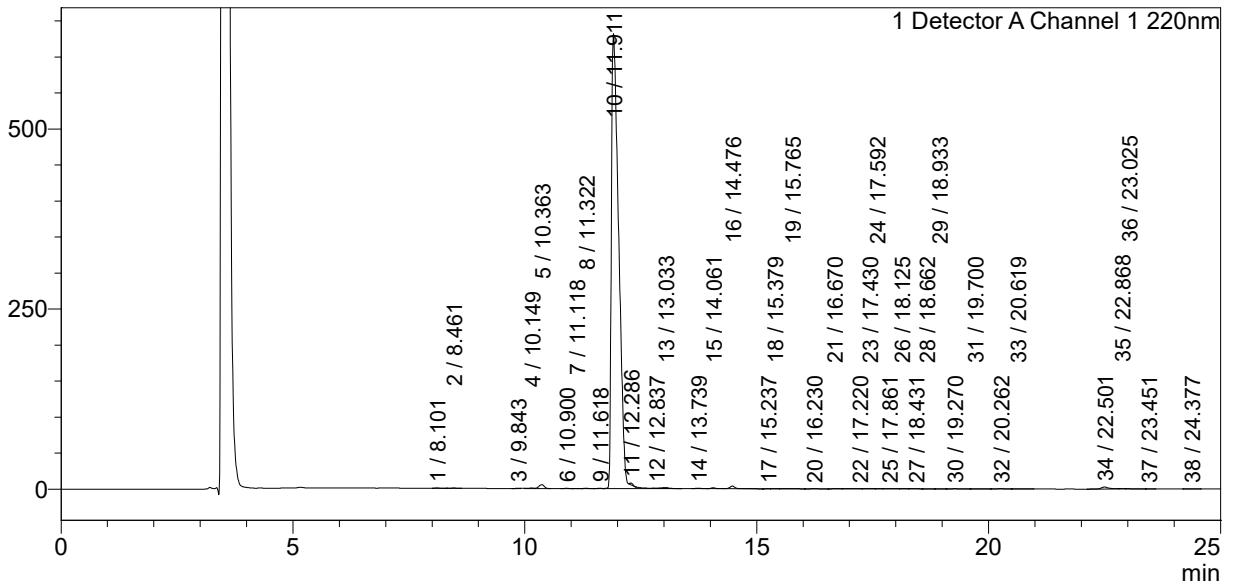

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.101	1905	328	0.026
2	8.461	2704	353	0.037
3	9.843	1177	152	0.016
4	10.149	5233	658	0.072
5	10.363	43112	5341	0.597
6	10.900	2590	409	0.036
7	11.118	1678	234	0.023
8	11.322	4028	555	0.056
9	11.618	3001	407	0.042
10	11.911	6967407	631767	96.429
11	12.286	10249	2368	0.142
12	12.837	1913	322	0.026
13	13.033	13113	1376	0.181
14	13.739	6047	608	0.084

Peak#	Ret. Time	Area	Height	Area%
15	14.061	8132	1237	0.113
16	14.476	29884	3607	0.414
17	15.237	1423	204	0.020
18	15.379	1961	207	0.027
19	15.765	5905	280	0.082
20	16.230	3326	188	0.046
21	16.670	3533	304	0.049
22	17.220	8816	490	0.122
23	17.430	8706	545	0.120
24	17.592	4692	511	0.065
25	17.861	8633	477	0.119
26	18.125	3288	295	0.046
27	18.431	4055	270	0.056
28	18.662	2926	214	0.040
29	18.933	1971	171	0.027
30	19.270	5077	288	0.070
31	19.700	2390	168	0.033
32	20.262	4193	453	0.058
33	20.619	2516	234	0.035
34	22.501	36773	2823	0.509
35	22.868	4251	493	0.059
36	23.025	6525	441	0.090
37	23.451	1194	141	0.017
38	24.377	1124	122	0.016
Total		7225453	659043	100.000