

Sample Name : β -Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E8772109I
 Time Processed :16:55:44
 Month-Day-Year Processed :09/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010009

Chromatogram

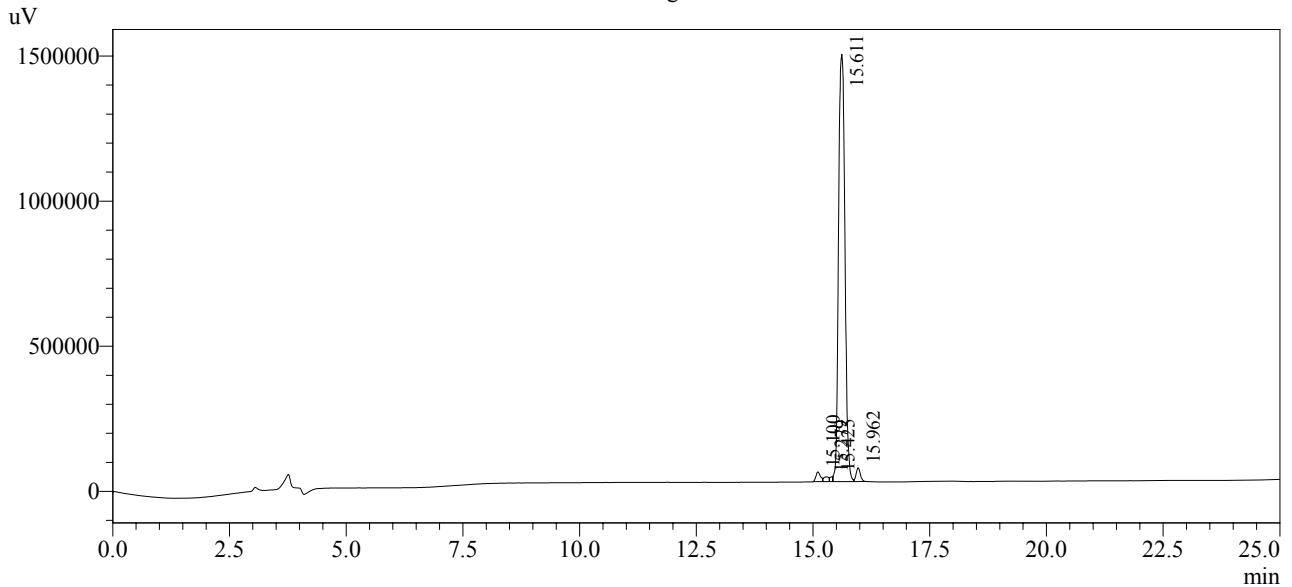

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.100	228710	33494	1.555
2	15.279	126523	16670	0.860
3	15.425	72505	18842	0.493
4	15.611	13981158	1472553	95.086
5	15.962	294733	47498	2.004
Total		14703628	1589058	100.000