

Sample Name :Amylin, human, amide
 Cat No. :RP11278
 Lot No. :E7328221C
 Time Processed :6:13:13 PM
 Month-Day-Year Processed :03/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

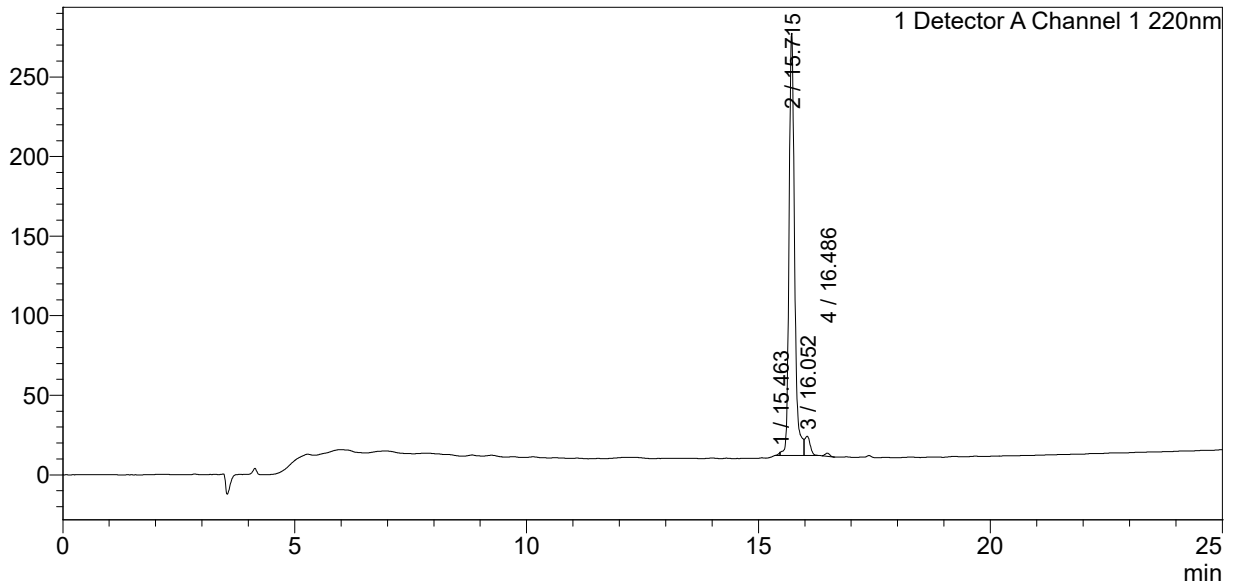

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.463	4670	1627	0.203
2	15.715	2187918	265357	95.060
3	16.052	96019	12030	4.172
4	16.486	13008	1941	0.565
Total		2301615	280955	100.000