

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E4525821A
 Time Processed :3:55:36
 Month-Day-Year Processed :01/07/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

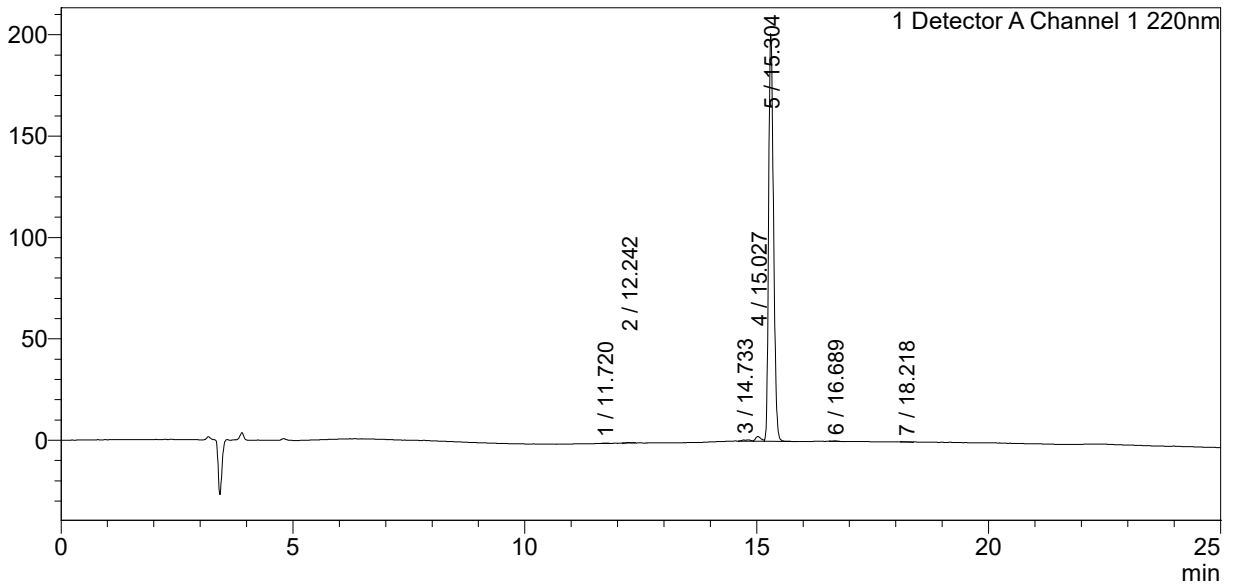

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.720	1541	213	0.102
2	12.242	2161	318	0.143
3	14.733	8175	549	0.540
4	15.027	19492	2289	1.287
5	15.304	1480277	187452	97.749
6	16.689	1852	273	0.122
7	18.218	869	120	0.057
Total		1514368	191215	100.000