

Sample Name :Melittin,honey bee
 Cat No. :RP20415
 Lot No. :E8735420J
 Time Processed :9:24:28
 Month-Day-Year Processed :10/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

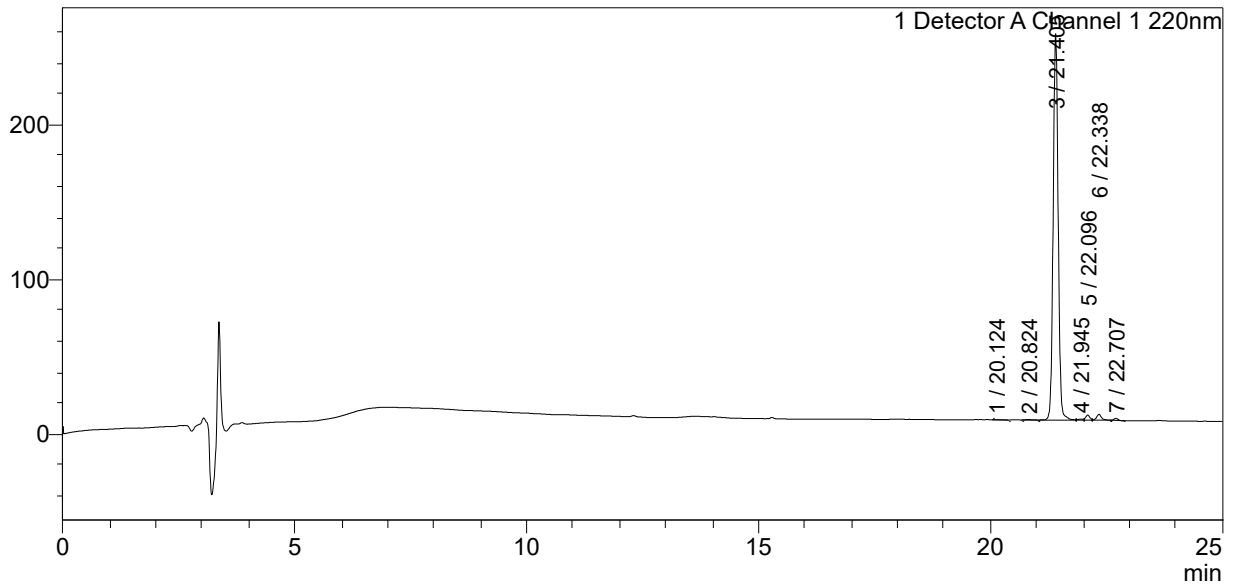

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	20.124	2064	162	0.107
2	20.824	3560	333	0.184
3	21.405	1864493	249748	96.510
4	21.945	4508	589	0.233
5	22.096	21628	3218	1.119
6	22.338	27625	3801	1.430
7	22.707	8037	1331	0.416
Total		1931914	259182	100.000