

Sample Name :Influenza A NP(366-374) Strain A/PR/8/35
 Cat No. :RP20267
 Lot No. :E1161620F
 Time Processed :7:57:27
 Month-Day-Year Processed :06/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

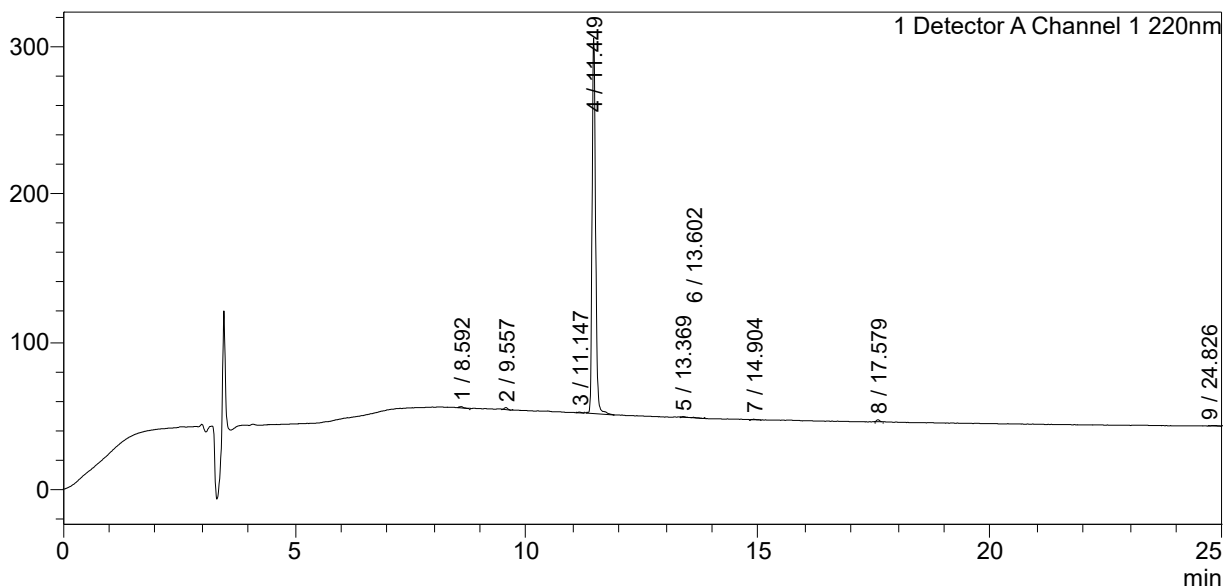

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.592	4635	934	0.339
2	9.557	6757	1493	0.494
3	11.147	2211	438	0.162
4	11.449	1336479	254169	97.790
5	13.369	2340	388	0.171
6	13.602	2443	338	0.179
7	14.904	2153	376	0.158
8	17.579	6311	1348	0.462
9	24.826	3348	427	0.245
Total		1366676	259911	100.000