

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E4570319K
 Time Processed :16:19:10
 Month-Day-Year Processed :11/13/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

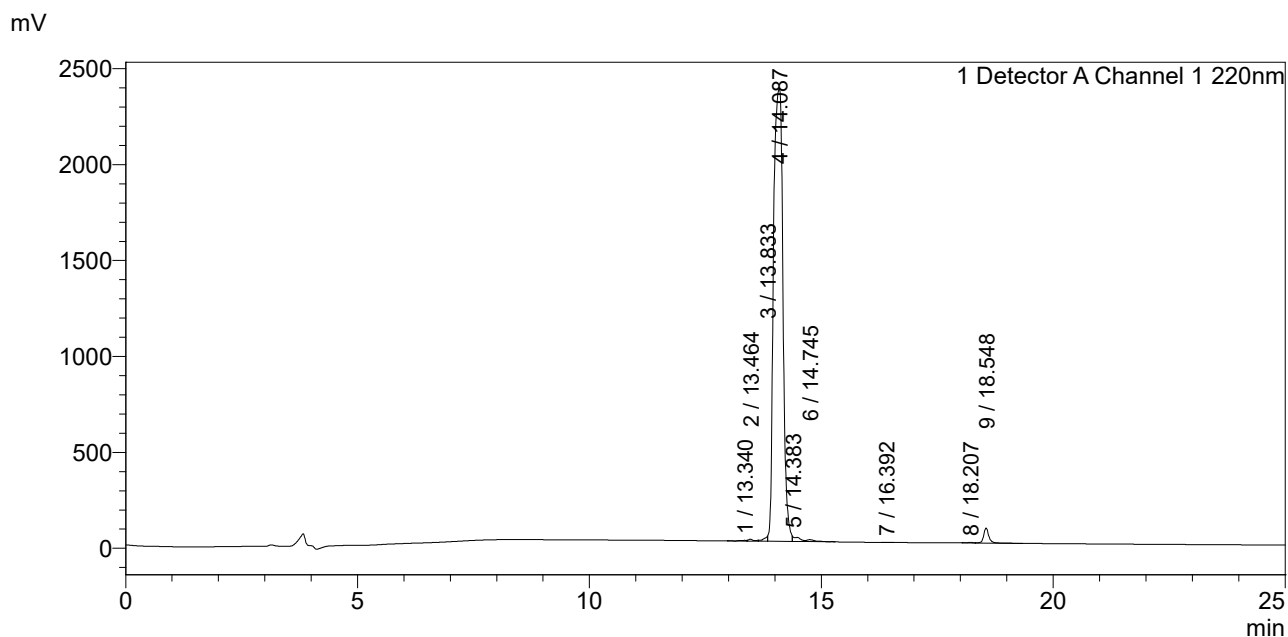

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.340	32856	3510	0.096
2	13.464	75980	9570	0.223
3	13.833	139685	23902	0.409
4	14.087	32881787	2362599	96.330
5	14.383	245143	25008	0.718
6	14.745	116970	9622	0.343
7	16.392	4679	746	0.014
8	18.207	21542	2326	0.063
9	18.548	615874	78201	1.804
Total		34134516	2515483	100.000