

Sample Name:C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat No. :RP11110
 Lot No. : E6814520H
 Time Processed: 11:28:20 AM
 Month-Day-Year Processed :08/05/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	20
25.00	Pumps	Pump A B.Conc	80
25.01	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	95
35.10	Pumps	Pump A B.Conc	20
40.20	Pumps	Pump A B.Conc	20
41.09	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

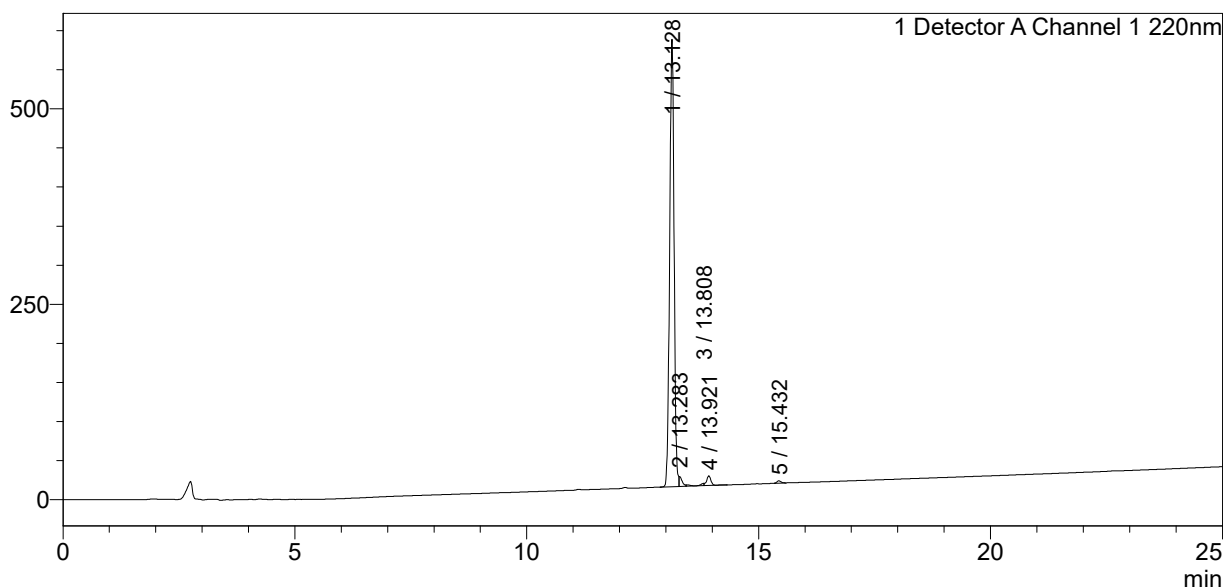

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.128	3783833	572515	95.537
2	13.283	55311	12781	1.397
3	13.808	25500	2828	0.644
4	13.921	79265	12404	2.001
5	15.432	16676	2833	0.421
Total		3960584	603360	100.000