

Sample Name :mTRP-2(180-188)  
 Cat No.: RP20250  
 Lot No.: PE6141901  
 Time Processed:14:32:15  
 Month-Day-Year Processed:01/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

### <Chromatogram>

mV

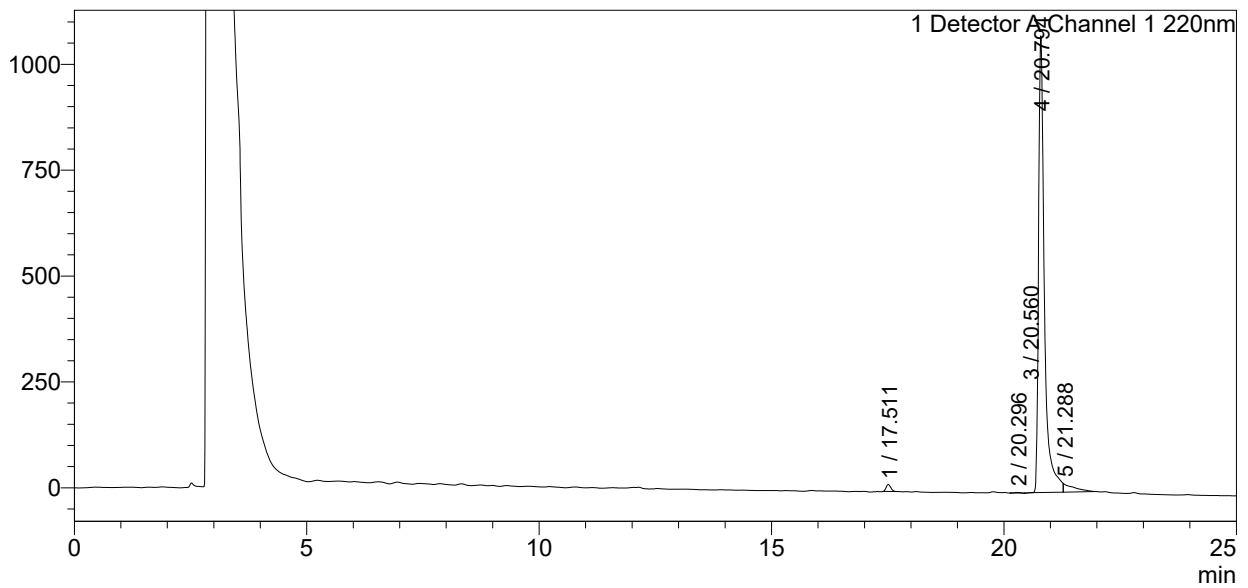

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.511	113225	16320	1.149
2	20.296	15420	1976	0.157
3	20.560	1962	436	0.020
4	20.794	9402742	1078299	95.451
5	21.288	317521	19984	3.223
Total		9850871	1117014	100.000