


# Mass Spectrum

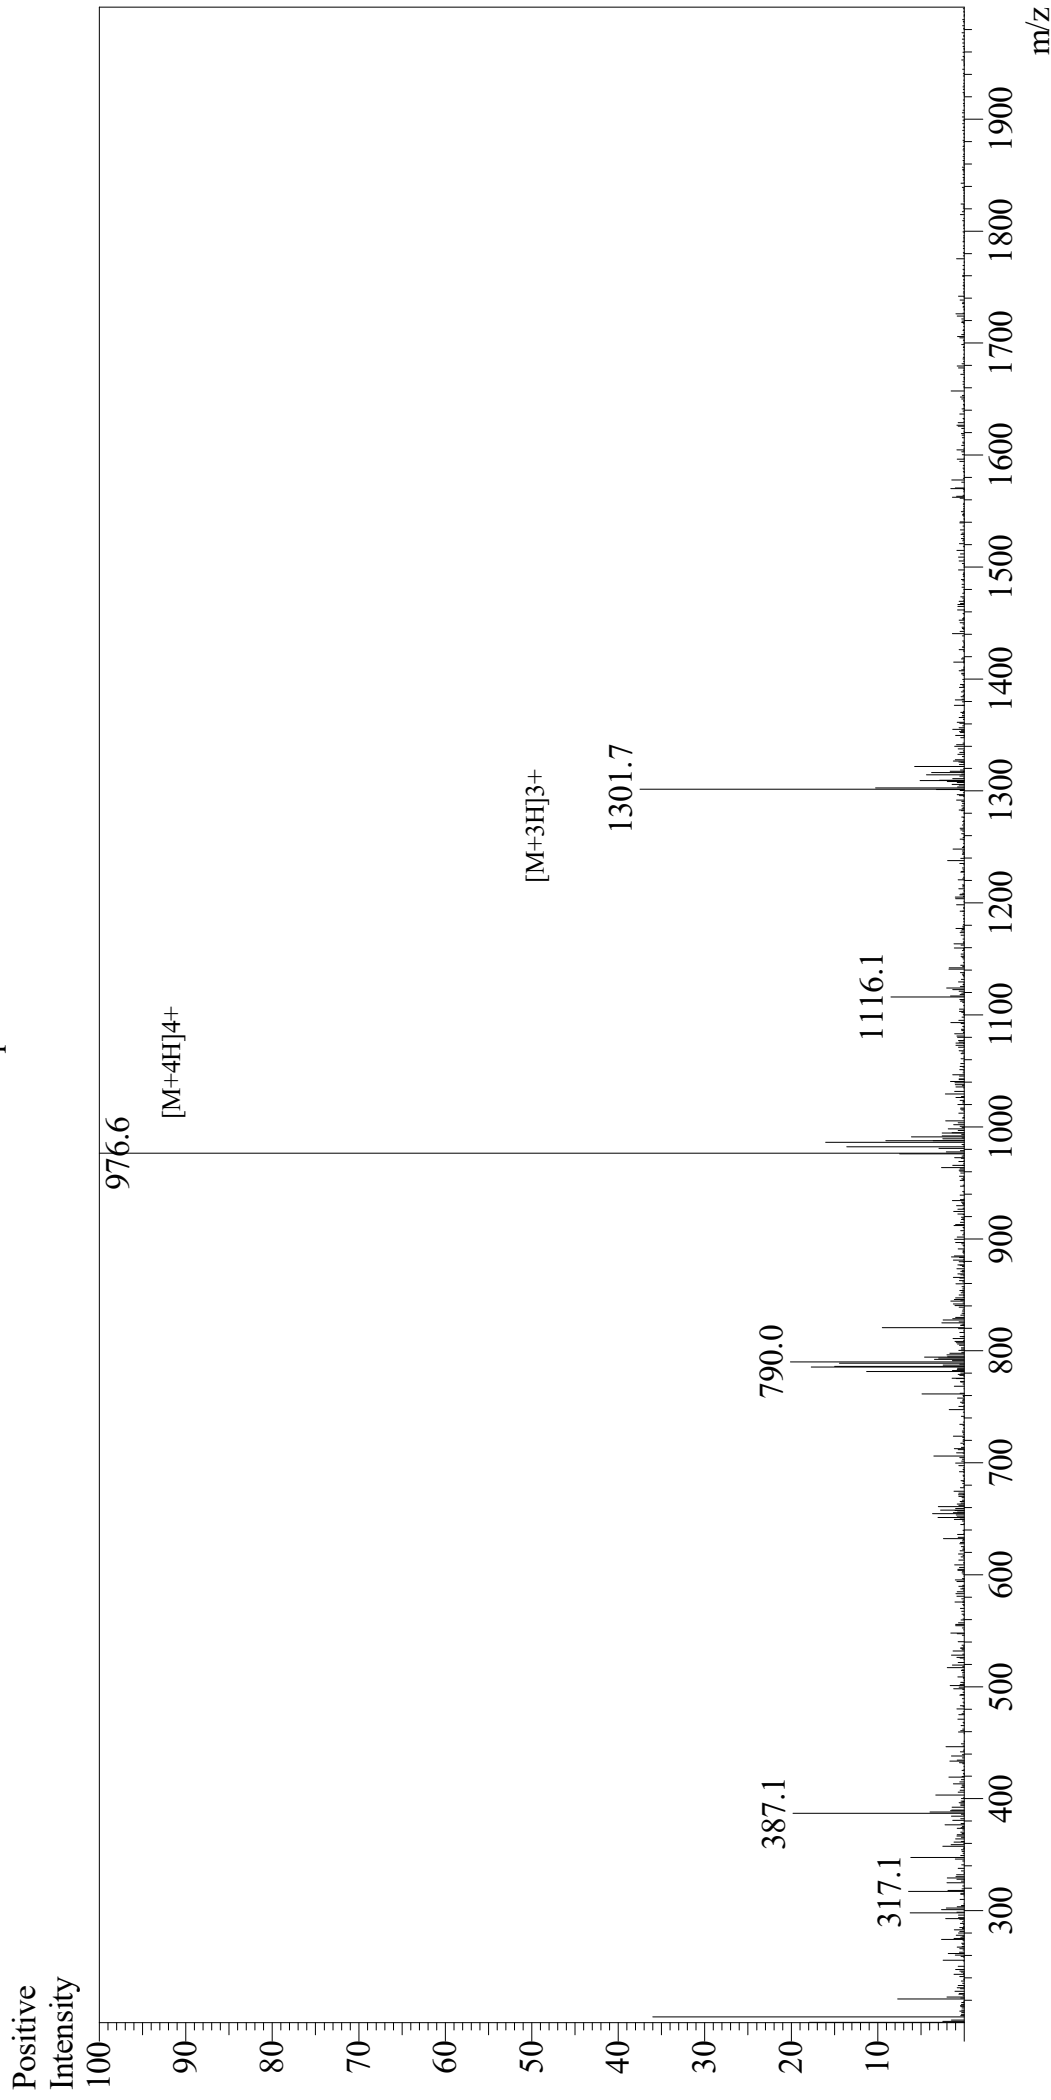

## Sample Information

User : Gary  
Month-Day Processed : 02/19/20  
Time Processed : 03:54:51 PM  
Injection Volume : 0.3  
Sample Name : Amylin, human, amide  
Cat No. : RP11278  
Lot No. : E6380720B  
Theoretical MW : 3903.28  
Observed MW : 3902.4

## Interface

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

## Equipment

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH