

Sample Name :Cys-TAT(47-57)
 Cat. No. : RP20343
 Lot. No. : PE8951902
 Time Processed : 18:08:00
 Month-Day-Year Processed : 03/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

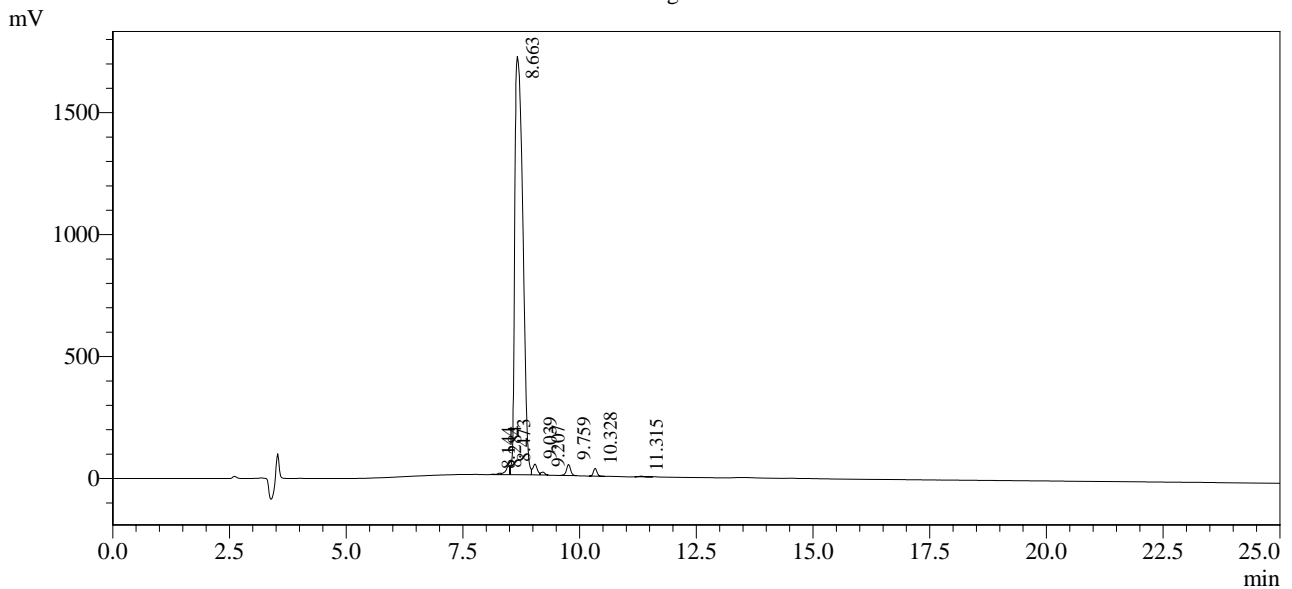

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.144	7749	1635	0.036
2	8.284	31989	6069	0.147
3	8.473	213386	34240	0.982
4	8.663	20641271	1716113	95.038
5	9.039	293395	43966	1.351
6	9.207	67376	11607	0.310
7	9.759	277413	44834	1.277
8	10.328	170936	31442	0.787
9	11.315	15556	2658	0.072
Total		21719070	1892564	100.000