

Sample Name :Jagged-1 (188-204)
 Cat. No. : RP20331
 Lot. No. :PE1921903
 Time Processed :17:38:29
 Month-Day-Year Processed :03/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

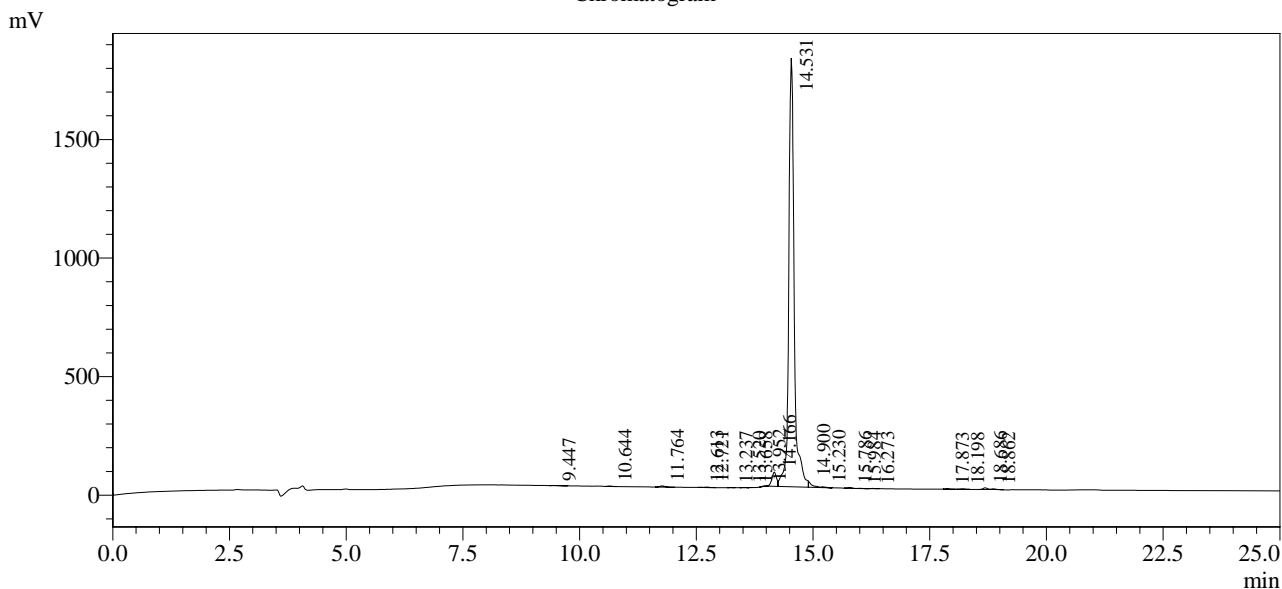

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.447	4796	746	0.031
2	10.644	9416	1800	0.061
3	11.764	38093	5053	0.247
4	12.613	3853	820	0.025
5	12.721	11292	2037	0.073
6	13.237	3622	826	0.024
7	13.520	3089	621	0.020
8	13.658	438	114	0.003
9	13.952	10265	2175	0.067
10	14.166	408708	59525	2.655
11	14.531	14647805	1807093	95.150
12	14.900	131287	26165	0.853
13	15.230	3873	805	0.025
14	15.786	19964	3367	0.130
15	15.984	5796	929	0.038
16	16.273	6919	1146	0.045
17	17.873	10133	1646	0.066
18	18.198	10301	1484	0.067
19	18.686	45689	6882	0.297
20	18.862	19035	2946	0.124
Total		15394373	1926180	100.000