

Sample Name :OVA Peptide (323-339)
 Cat. No. : RP10610
 Lot. No. : E3432820E
 Time Processed :14:25:53
 Month-Day-Year Processed :05/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

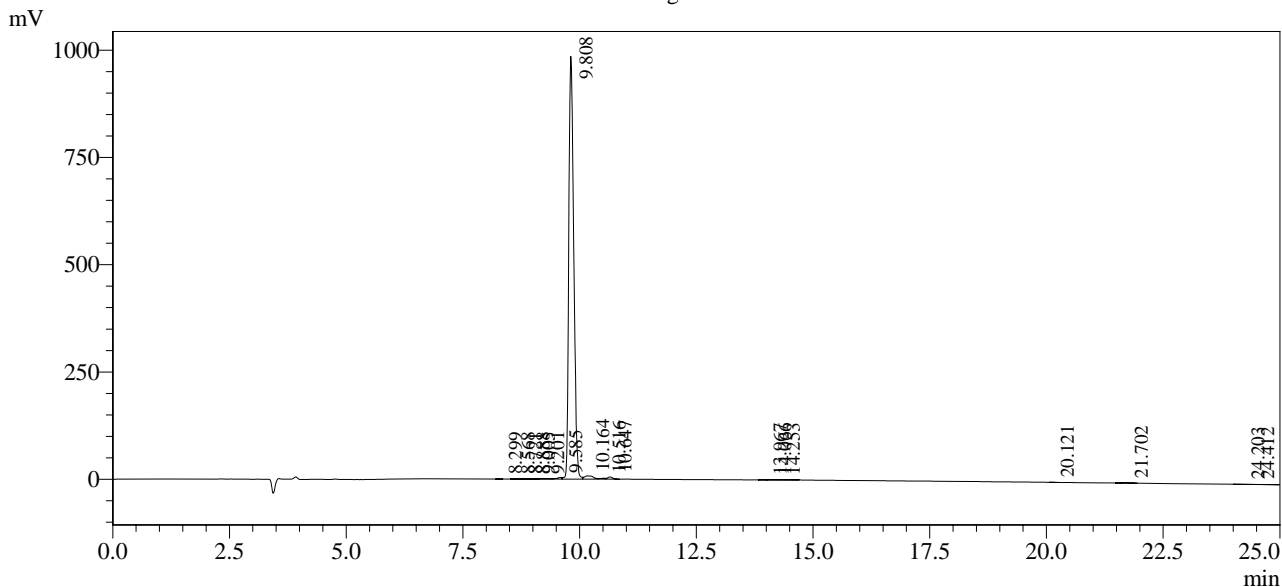

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.299	1042	153	0.014
2	8.568	1181	204	0.016
3	8.721	2477	287	0.033
4	8.888	1370	235	0.018
5	9.005	1948	294	0.026
6	9.201	6549	605	0.087
7	9.585	30105	3735	0.402
8	9.808	7258636	985491	96.877
9	10.164	97533	7408	1.302
10	10.516	15779	1951	0.211
11	10.647	36377	4899	0.486
12	13.967	1363	171	0.018
13	14.066	1566	269	0.021
14	14.253	10556	448	0.141
15	20.121	1431	225	0.019
16	21.702	6768	443	0.090
17	24.203	4484	350	0.060
18	24.412	13444	589	0.179
Total		7492610	1007754	100.000