

Sample Name :OVA Peptide (323-339)

Cat. No. : RP10610

Lot. No. : E9191621C

Time Processed :5:37:38

Month-Day-Year Processed :03/29/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

### <Chromatogram>

mV

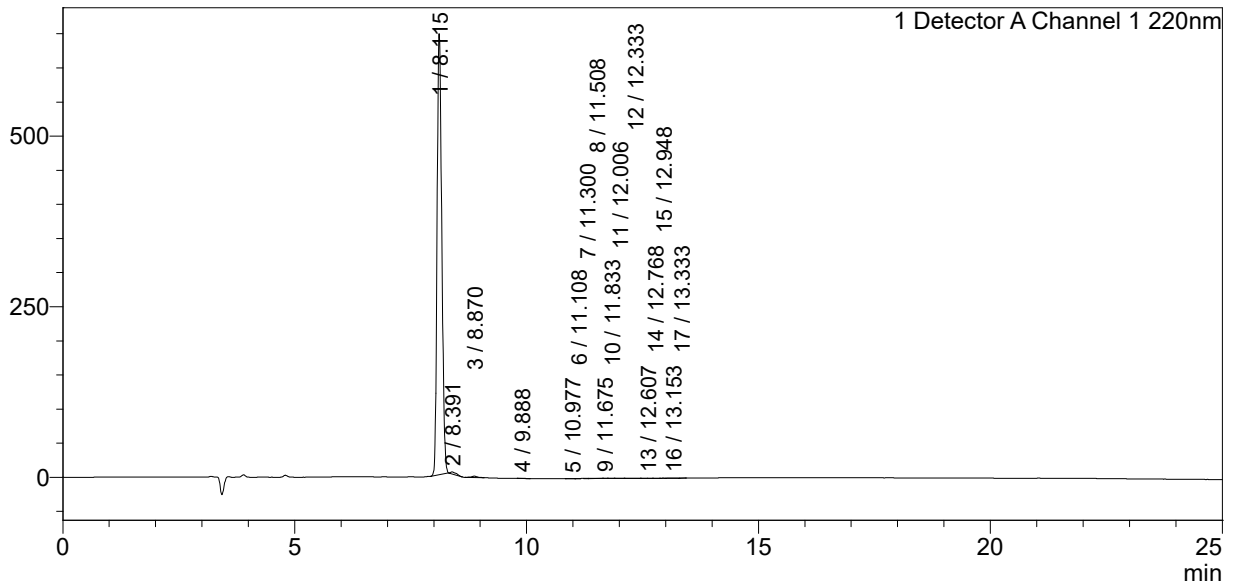

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.115	4547860	646568	98.738
2	8.391	26968	2977	0.586
3	8.870	15895	1910	0.345
4	9.888	1072	157	0.023
5	10.977	634	79	0.014
6	11.108	249	56	0.005
7	11.300	452	97	0.010
8	11.508	1600	112	0.035
9	11.675	415	84	0.009
10	11.833	692	94	0.015
11	12.006	1486	153	0.032
12	12.333	2485	131	0.054
13	12.607	2242	171	0.049
14	12.768	819	130	0.018
15	12.948	596	109	0.013
16	13.153	2376	274	0.052

Peak#	Ret. Time	Area	Height	Area%
17	13.333	161	35	0.003
Total		4606002	653135	100.000