


Mass Spectrum

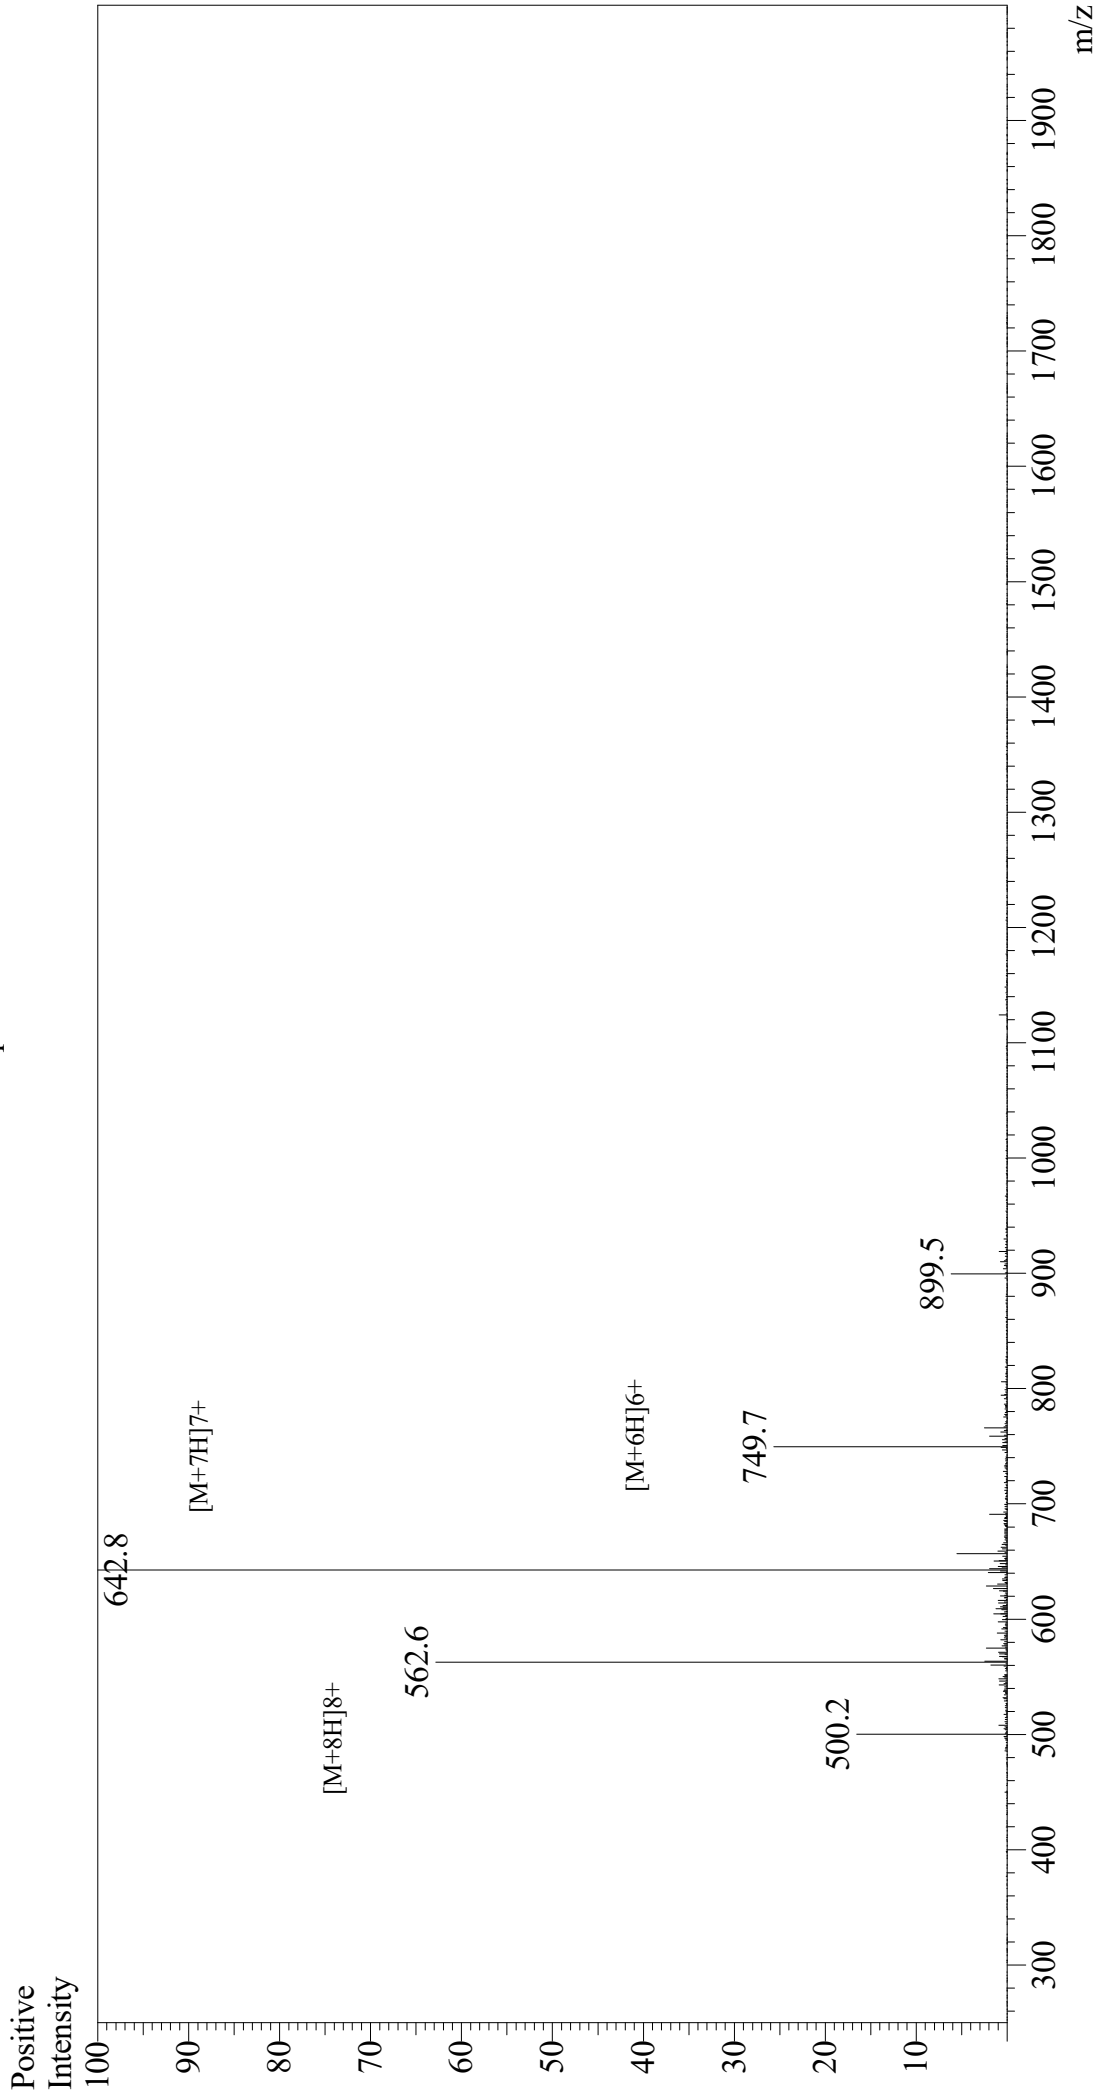

Sample Information
Month-Day Processed : 07/17/21
Time Processed : 7:12:10
Injection Volume : 0.4
Sample Name : LL-37, scrambled
Cat No. : RP20332
Lot No. : E4118921G
Theoretical MW : 4493.30
Observed MW : 4492.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH