

Sample Name :β-Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E5729819K
 Time Processed :8:15:16
 Month-Day-Year Processed : 11/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

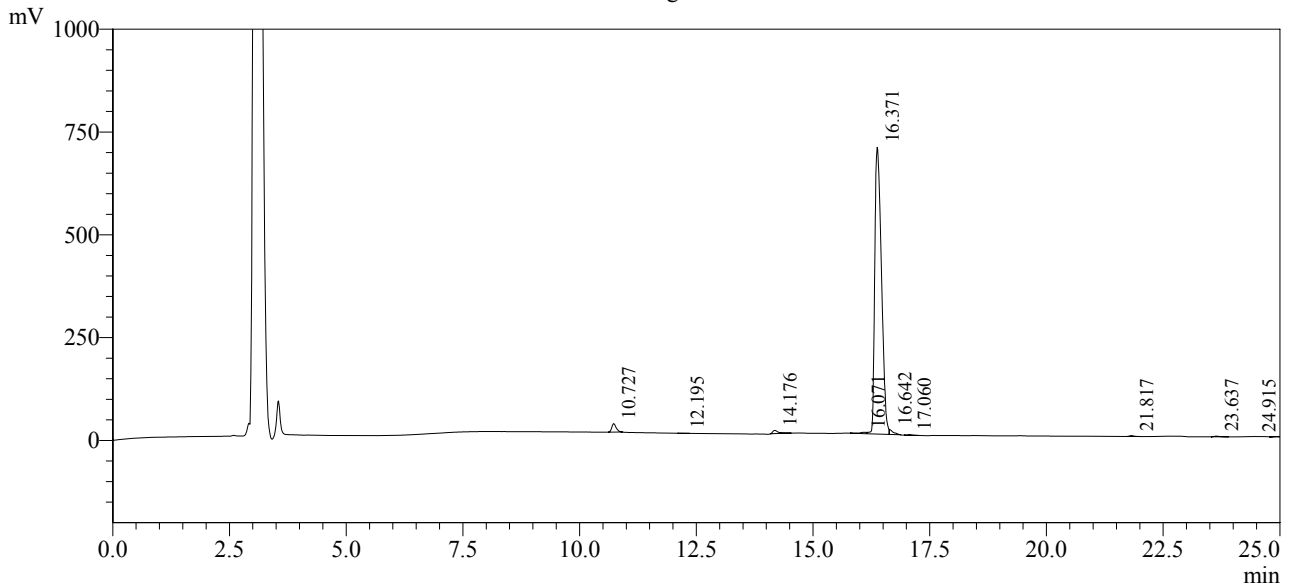

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.727	134982	20503	1.847
2	12.195	3117	444	0.043
3	14.176	66007	8026	0.903
4	16.071	29121	2989	0.399
5	16.371	6965256	697394	95.325
6	16.642	67557	11945	0.925
7	17.060	7148	1090	0.098
8	21.817	13802	2141	0.189
9	23.637	13173	1720	0.180
10	24.915	6682	946	0.091
Total		7306844	747199	100.000