

Sample Name :IRBP (1 - 20), human  
 Cat No.: RP20269  
 Lot No.: E6823120H  
 Time Processed :10:34:13  
 Month-Day-Year Processed :08/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

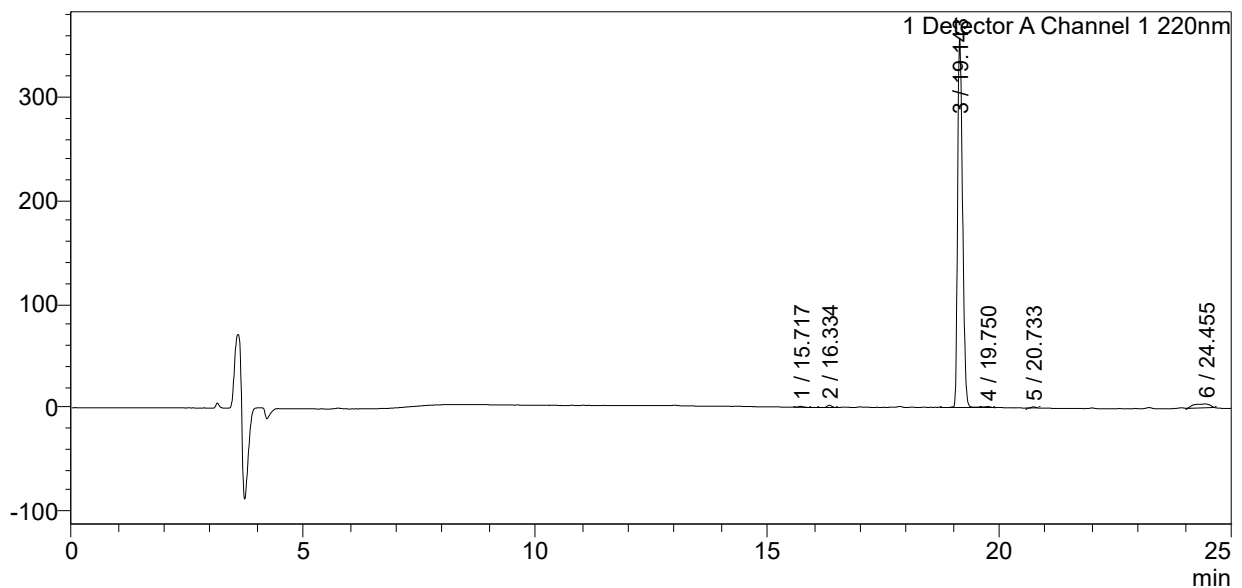

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.717	6362	936	0.229
2	16.334	13034	2188	0.468
3	19.143	2659212	356917	95.515
4	19.750	9472	988	0.340
5	20.733	6829	1144	0.245
6	24.455	89156	3426	3.202
Total		2784064	365600	100.000