

Sample Name : c-Myc Peptide
 Cat. No. : RP11731
 Lot. No. : PE5381611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

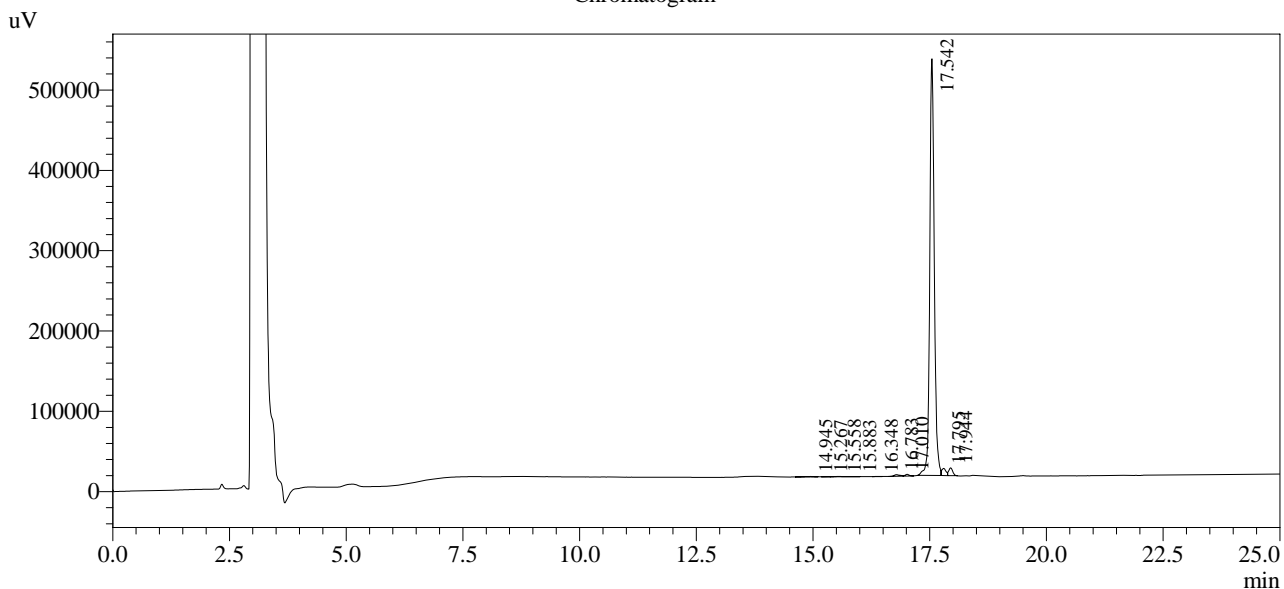

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.945	7342	501	0.202
2	15.267	1466	149	0.040
3	15.558	5411	416	0.149
4	15.883	1537	122	0.042
5	16.348	1027	146	0.028
6	16.783	17965	1964	0.493
7	17.010	12367	2082	0.340
8	17.542	3482266	518530	95.617
9	17.795	56673	8926	1.556
10	17.944	55838	9703	1.533
Total		3641892	542539	100.000