


# Mass Spectrum

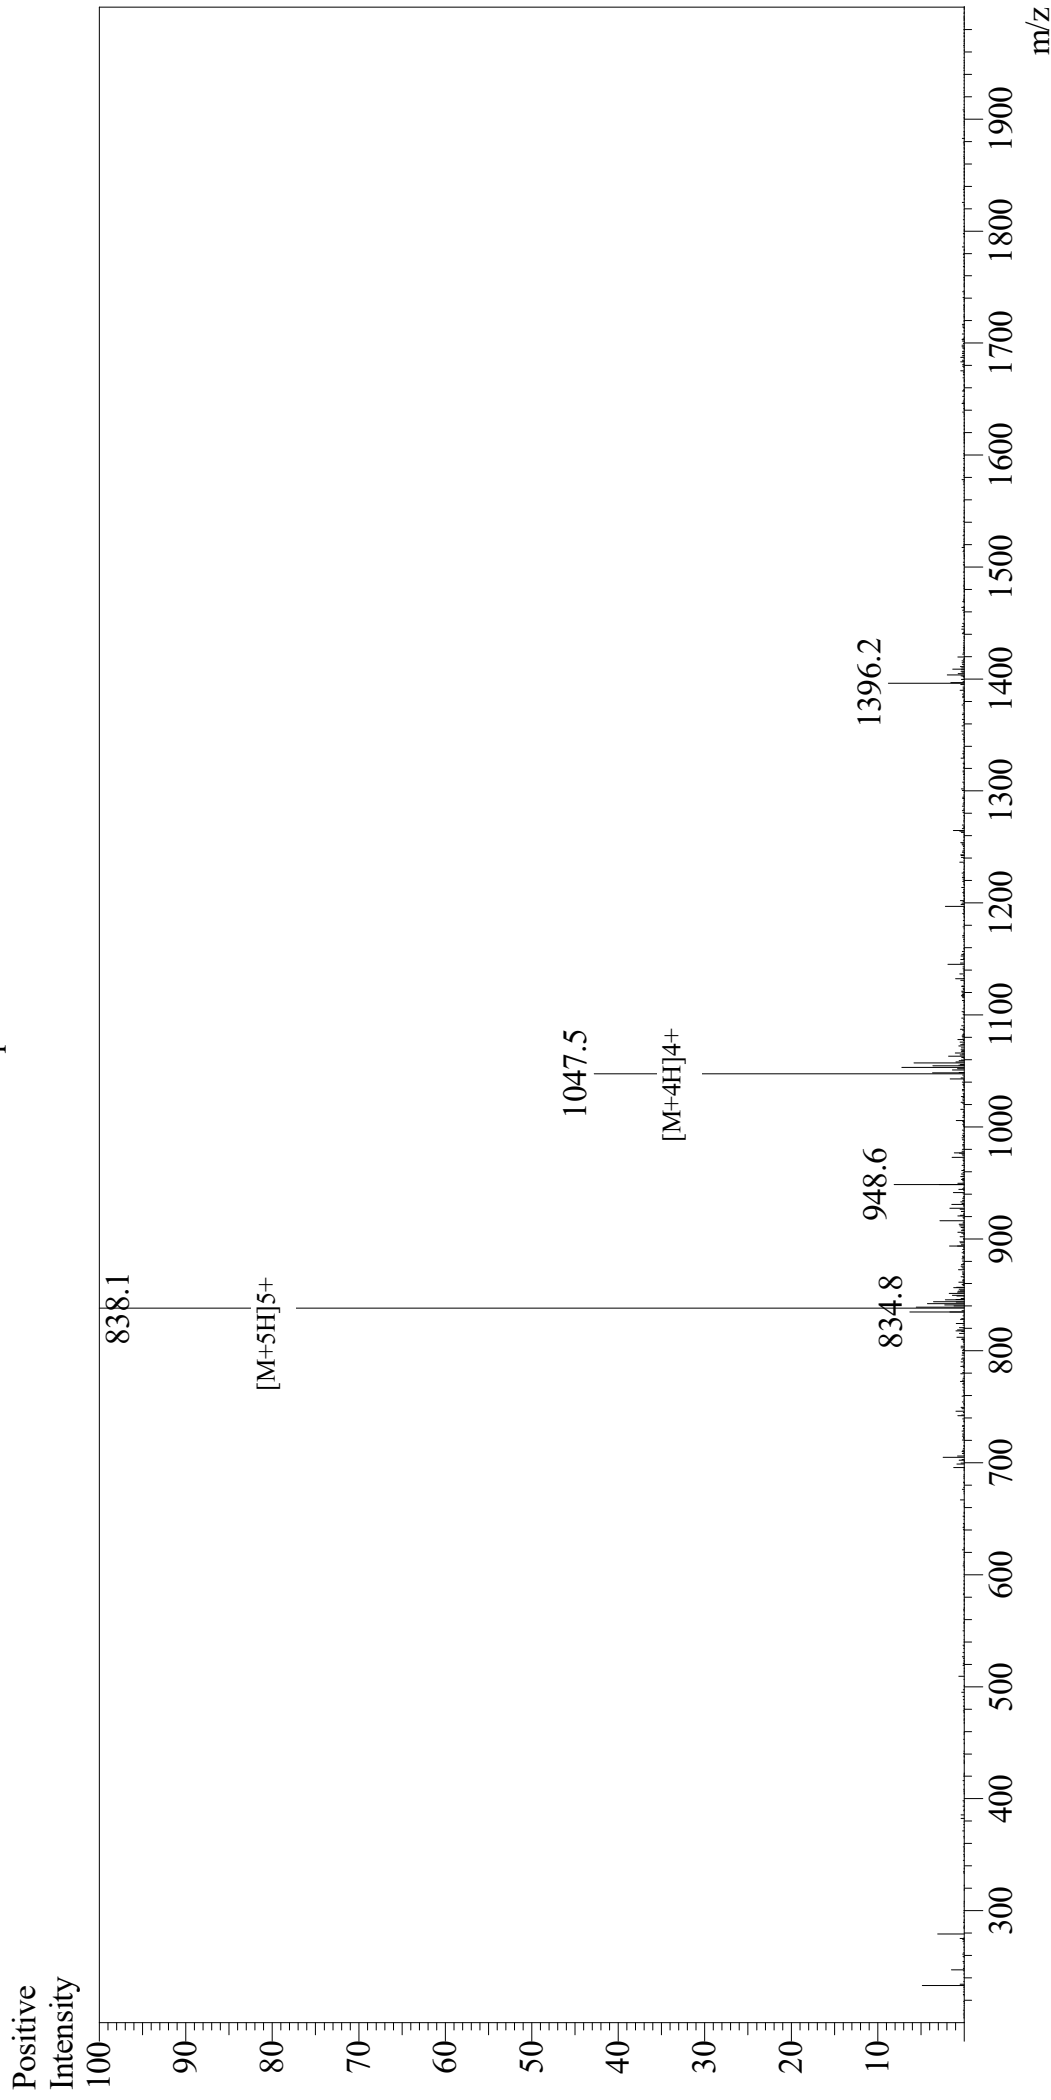

## Sample Information

User : Gary  
Month-Day Processed : 03/11/19  
Time Processed : 12:28:39 PM  
Injection Volume : 0.2  
Sample Name : Exendin-4  
Cat No. : RP10874  
Lot No. : PE7941902  
Theoretical MW : 4186.66  
Observed MW : 4185.5

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH