

Sample Name : Rabies Virus Glycoprotein  
 Cat No. : RP20464 Lot No. : PE2691806

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


| Time  | Unit       | Command       | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01  | Pumps      | Pump A B.Conc | 5     |         |
| 25.00 | Pumps      | Pump A B.Conc | 65    |         |
| 25.01 | Pumps      | Pump A B.Conc | 95    |         |
| 27.00 | Pumps      | Pump A B.Conc | 95    |         |
| 27.01 | Pumps      | Pump A B.Conc | 5     |         |
| 35.00 | Pumps      | Pump A B.Conc | 5     |         |
| 35.01 | Controller | Stop          |       |         |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

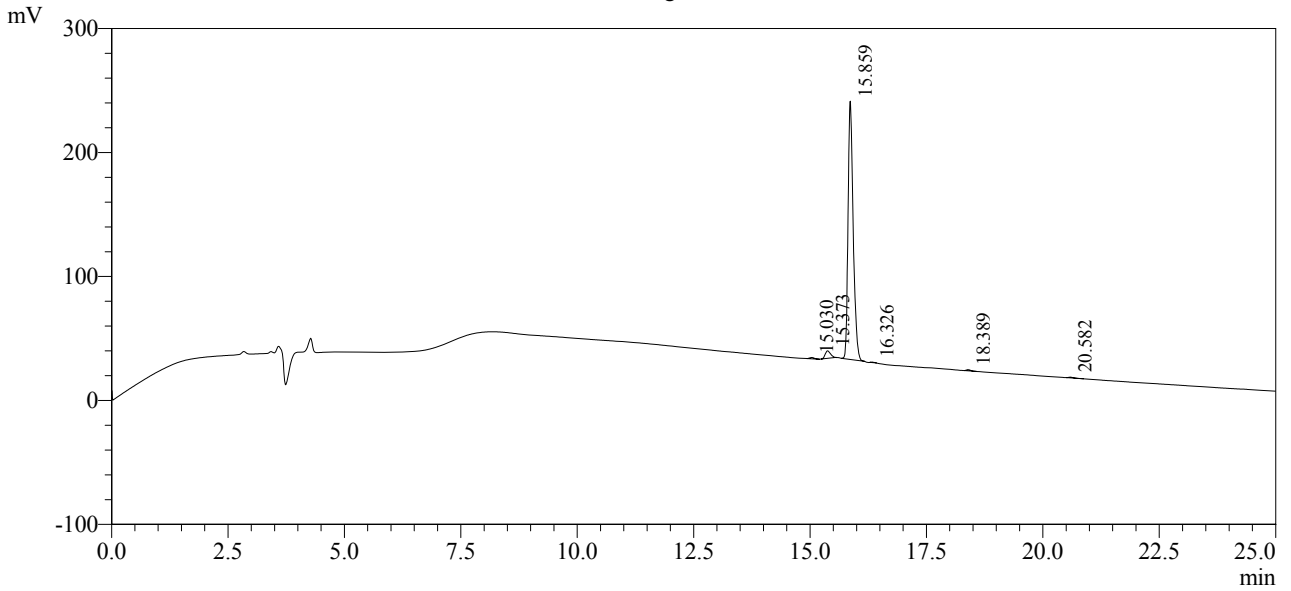

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area    | Height | Area %  |
|-------|-----------|---------|--------|---------|
| 1     | 15.030    | 7054    | 1049   | 0.424   |
| 2     | 15.373    | 48503   | 6083   | 2.913   |
| 3     | 15.859    | 1598189 | 208347 | 95.984  |
| 4     | 16.326    | 1831    | 401    | 0.110   |
| 5     | 18.389    | 5630    | 950    | 0.338   |
| 6     | 20.582    | 3851    | 573    | 0.231   |
| Total |           | 1665057 | 217402 | 100.000 |