

Sample Name : Glucagon (1-29), Human
 Cat. No. : RP10772
 Lot. No. : E0093319L
 Time Processed :9:57:57
 Month-Day-Year Processed :12/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

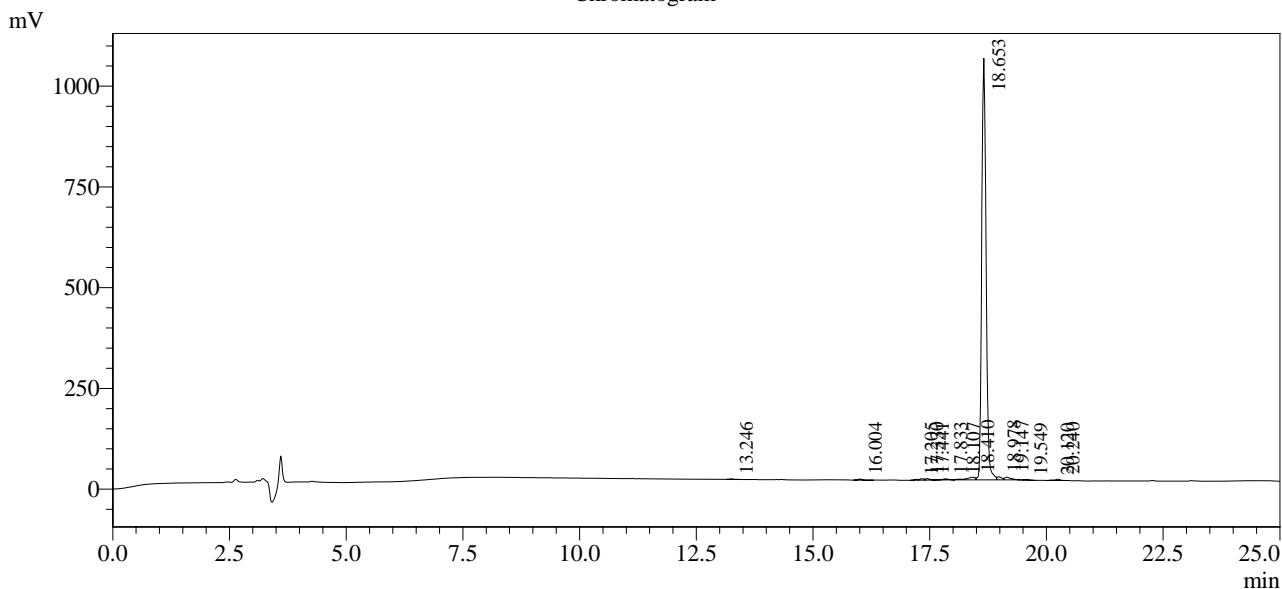

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.246	9217	1393	0.128
2	16.004	14827	2540	0.206
3	17.205	12113	2030	0.168
4	17.330	23322	3741	0.324
5	17.441	24663	3739	0.342
6	17.833	26107	2930	0.362
7	18.107	14097	1797	0.196
8	18.410	77107	6674	1.070
9	18.653	6855163	1046307	95.105
10	18.978	52573	7747	0.729
11	19.147	62435	6656	0.866
12	19.549	6836	1002	0.095
13	20.120	7727	1328	0.107
14	20.240	21818	3349	0.303
Total		7208005	1091234	100.000