

Sample Name :Cortistatin 14, human, rat  
 Cat. No. : RP10972  
 Lot. No. : PE2141906  
 Time Processed :8:50:58  
 Month-Day-Year Processed :06/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

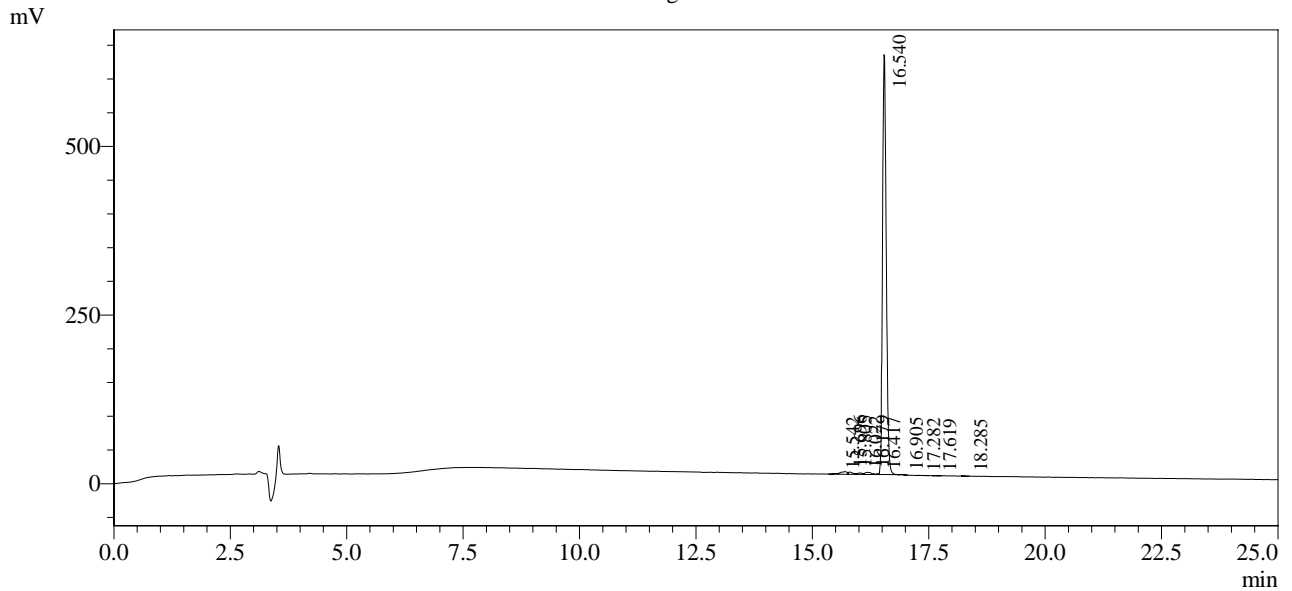

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.542	7442	1063	0.208
2	15.696	37498	3895	1.047
3	15.805	21889	3220	0.611
4	16.022	16114	2125	0.450
5	16.179	28971	3160	0.809
6	16.417	5734	973	0.160
7	16.540	3458028	622406	96.512
8	16.905	2999	527	0.084
9	17.282	2213	234	0.062
10	17.619	1030	198	0.029
11	18.285	1074	240	0.030
Total		3582993	638041	100.000