


Mass Spectrum

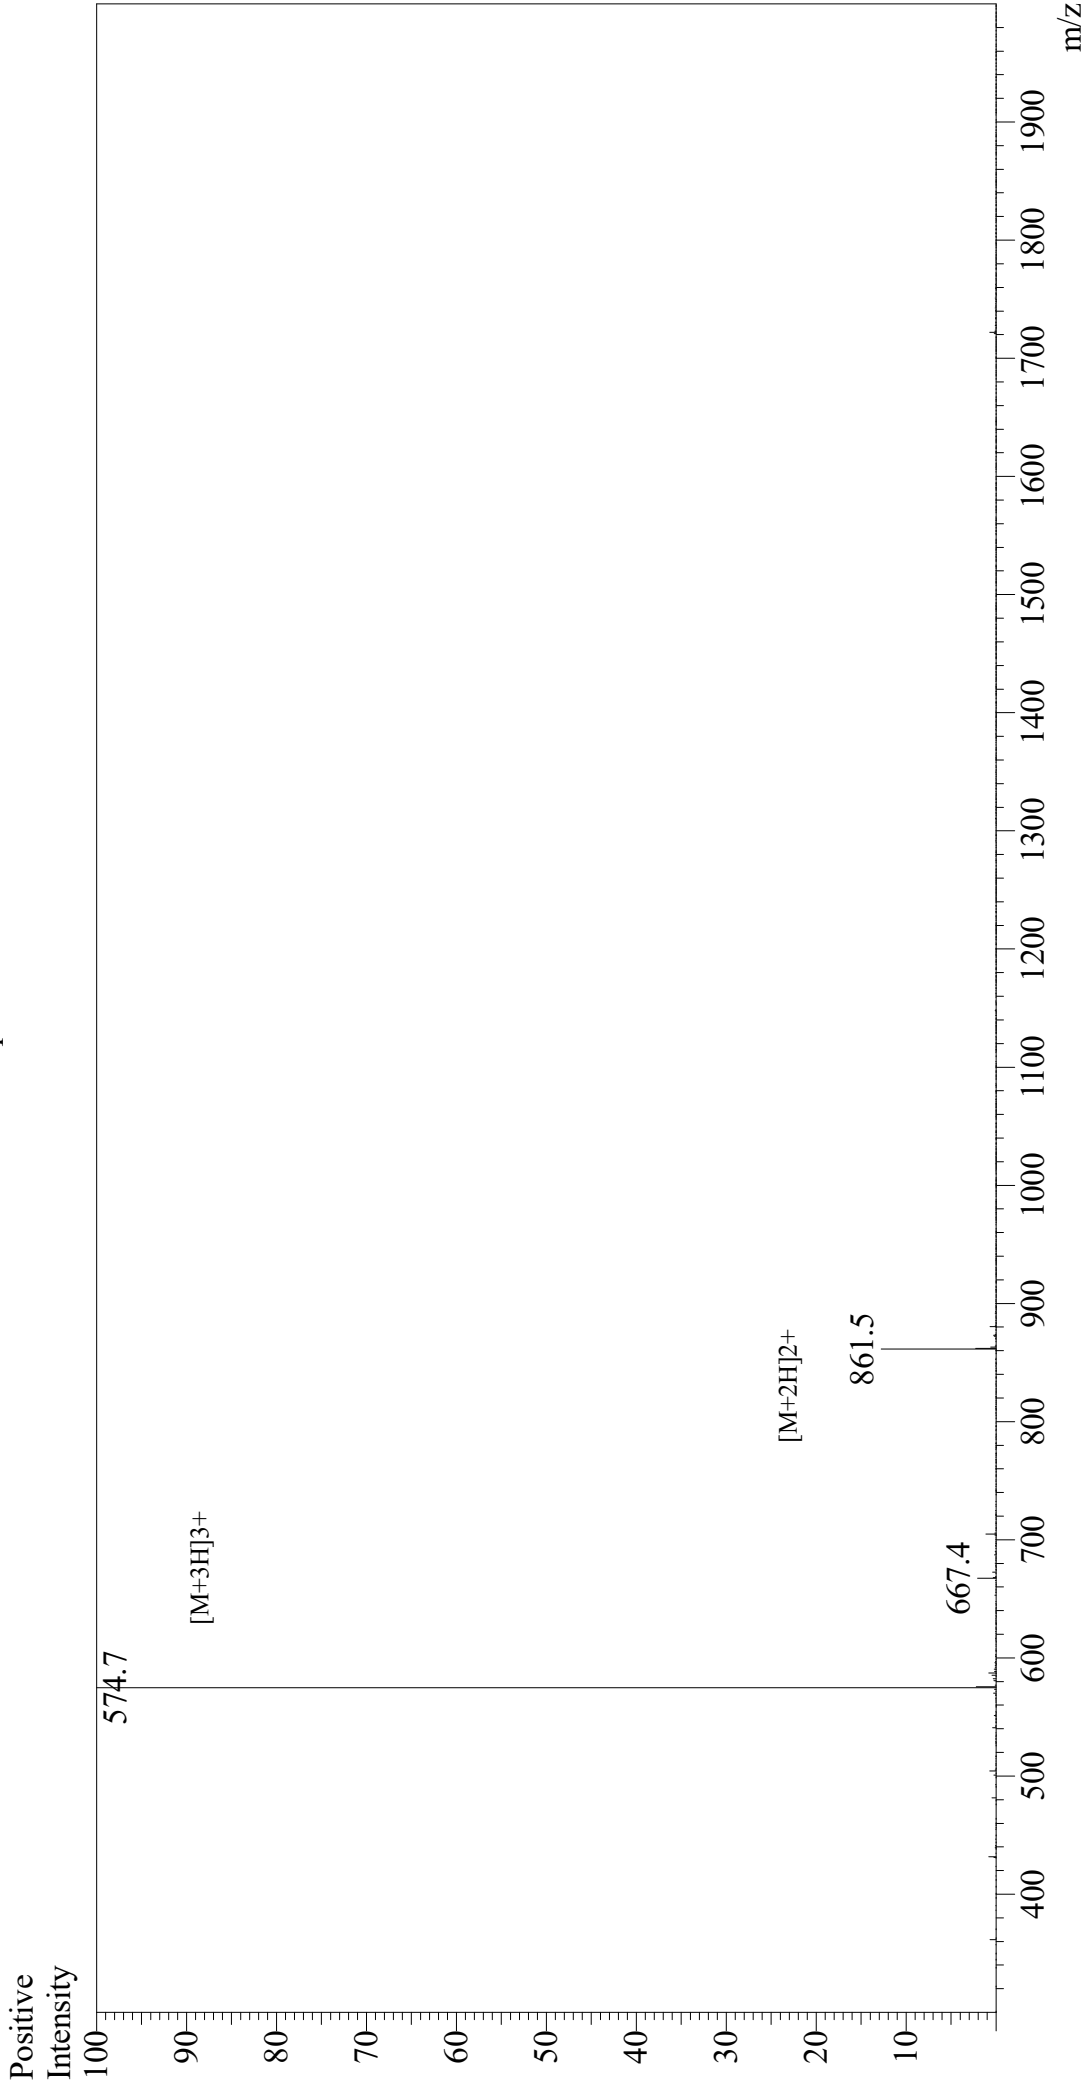

Sample Information

Acquired by : Gary
Month-Day Processed : 06/17/19
Time Processed : 10:01:51 PM
Injection Volume : 0.4
Sample Name : Cortistatin 14, human, rat
Cat. No. : RP10972
Lot. No. : PE2141906
Theoretical MW : 1721.01
Observed MW : 1721.1

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH