

Sample Name: IRBP (1-20), human  
 Cat No. : RP20269  
 Lot No. : E3594720B  
 Time Processed: 2:23:58 PM  
 Month-Day-Year Processed :02/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

### <Chromatogram>

mV

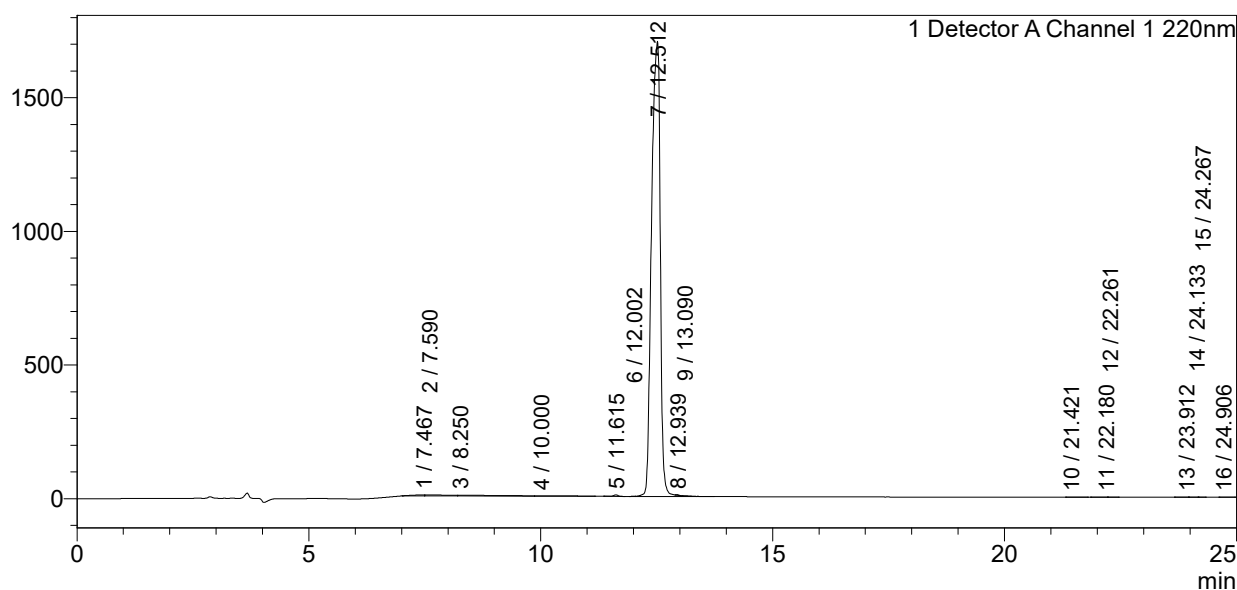

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.467	73291	3639	0.323
2	7.590	139830	3706	0.616
3	8.250	202795	2870	0.893
4	10.000	62720	1476	0.276
5	11.615	36846	5677	0.162
6	12.002	5286	1079	0.023
7	12.512	22155845	1702990	97.613
8	12.939	7044	1788	0.031
9	13.090	2496	521	0.011
10	21.421	1912	120	0.008
11	22.180	3047	240	0.013
12	22.261	1970	230	0.009
13	23.912	1010	109	0.004
14	24.133	1222	117	0.005

Peak#	Ret. Time	Area	Height	Area%
15	24.267	1128	131	0.005
16	24.906	1131	70	0.005
Total		22697572	1724763	100.000