

Sample Name : CEF20
 Cat. No. : RP11781
 Lot. No. : PE9821905
 Time Processed :14:11:43
 Month-Day-Year Processed :05/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.10	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

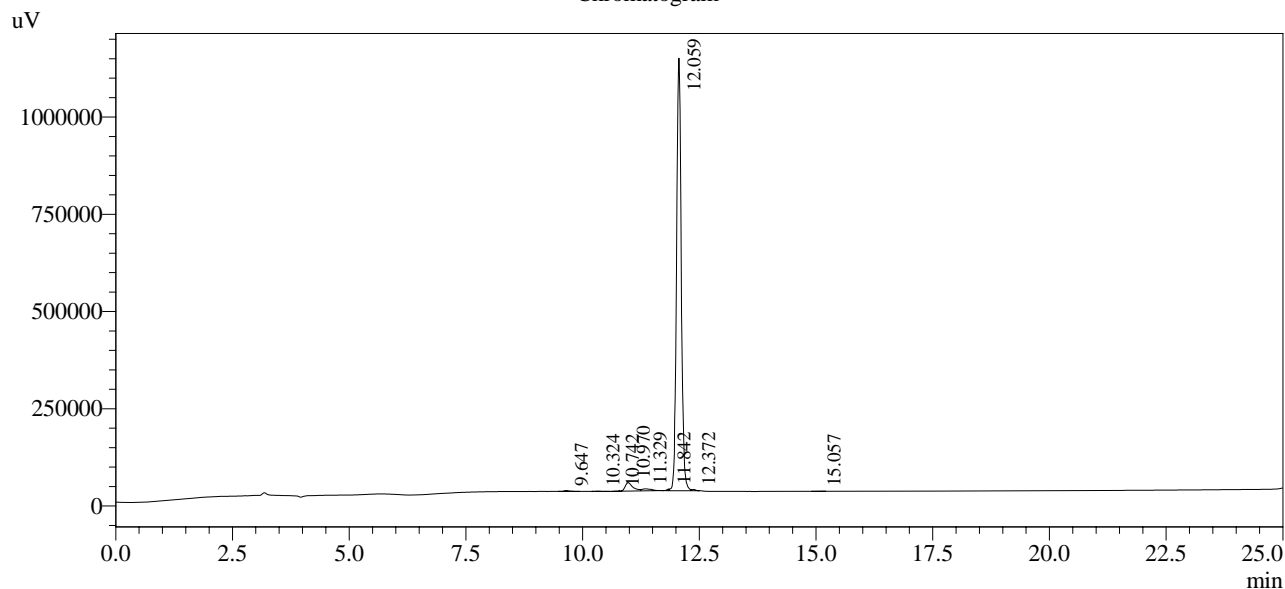

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.647	15381	1940	0.188
2	10.324	3586	391	0.044
3	10.742	1131	177	0.014
4	10.970	252477	22119	3.083
5	11.329	76547	5390	0.935
6	11.842	13652	4054	0.167
7	12.059	7802323	1111097	95.267
8	12.372	18966	3268	0.232
9	15.057	5877	823	0.072
Total		8189940	1149258	100.000