

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat No. :RP10795
 Lot No. :E5624120K
 Time Processed : 9:17:08
 Month-Day-Year Processed : 11/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

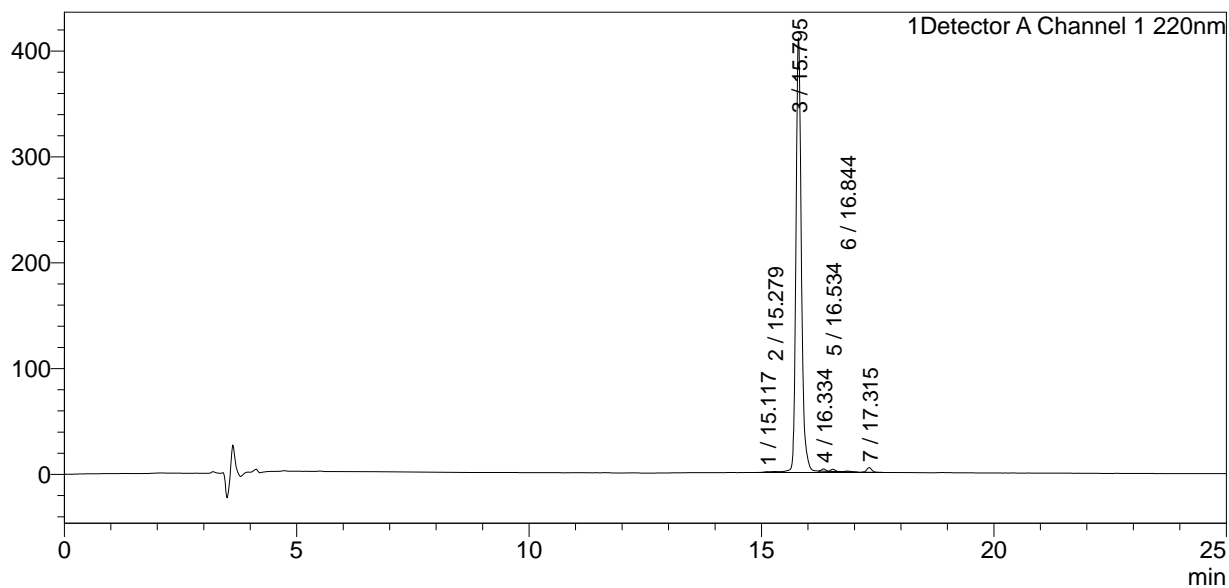

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.117	6470	737	0.187
2	15.279	8466	917	0.245
3	15.795	3381267	410287	97.673
4	16.334	12923	2125	0.373
5	16.534	13295	2056	0.384
6	16.844	6401	679	0.185
7	17.315	32990	4398	0.953
Total		3461812	421201	100.000