

Sample Name :Amylin, human, amide  
 Cat. No. : RP11278  
 Lot. No. : E2271120J  
 Time Processed : 11:11:40 AM  
 Month-Day-Year Processed : 10/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
45.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010017

mV

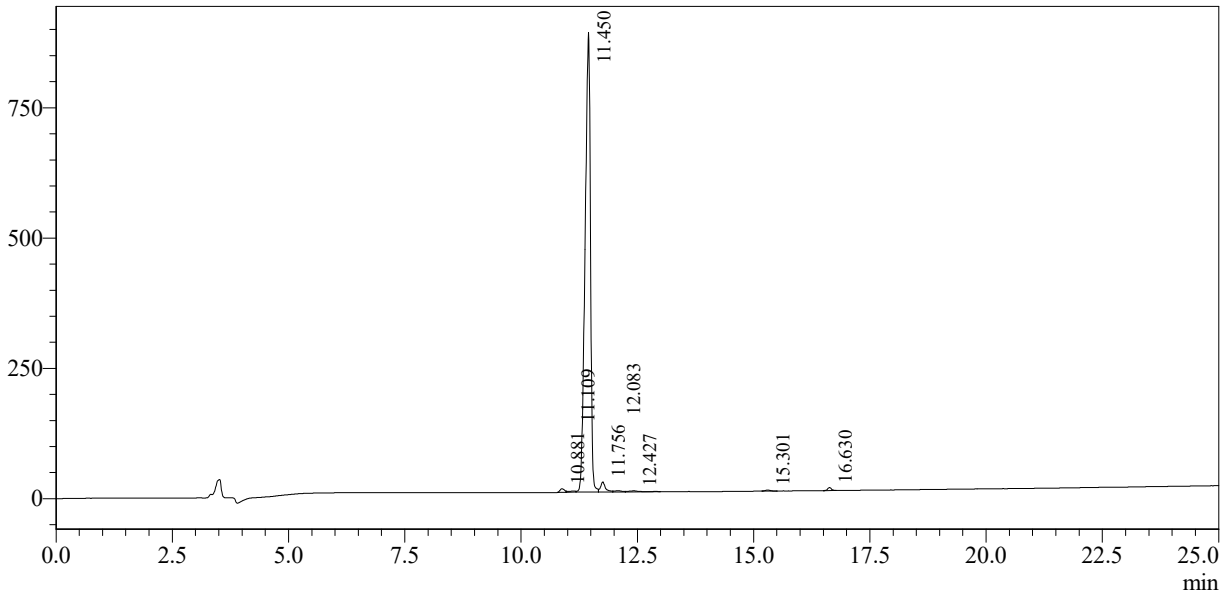

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.881	43893	6755	0.594
2	11.109	23220	2212	0.314
3	11.450	7067938	881463	95.716
4	11.756	141306	19532	1.914
5	12.083	27564	2244	0.373
6	12.427	36662	2156	0.496
7	15.301	14066	1959	0.190
8	16.630	29669	5510	0.402
Total		7384318	921832	100.000