

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. :RP11529
 Lot No. :E7240720B
 Time Processed :23:10:07
 Month-Day-Year Processed :02/01/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

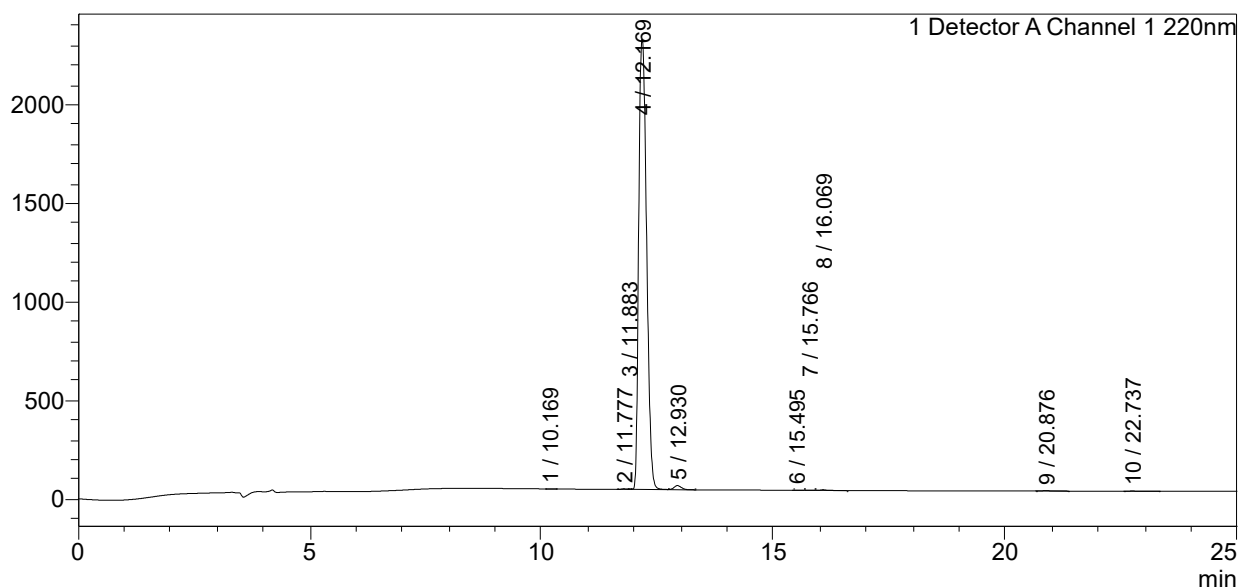

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.169	2573	435	0.009
2	11.777	22100	3213	0.081
3	11.883	9624	1923	0.035
4	12.169	26935261	2286075	98.789
5	12.930	219134	20522	0.804
6	15.495	2171	363	0.008
7	15.766	2220	377	0.008
8	16.069	32485	3521	0.119
9	20.876	28662	2159	0.105
10	22.737	11138	718	0.041
Total		27265369	2319306	100.000