

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : E6969619J  
 Time Processed : 13:22:45  
 Month-Day-Year Processed : 12/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
29.00	Pumps	Pump A B.Conc	95	
29.01	Pumps	Pump A B.Conc	5	
34.00	Pumps	Pump A B.Conc	5	
34.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : SS-CM-0310

Chromatogram

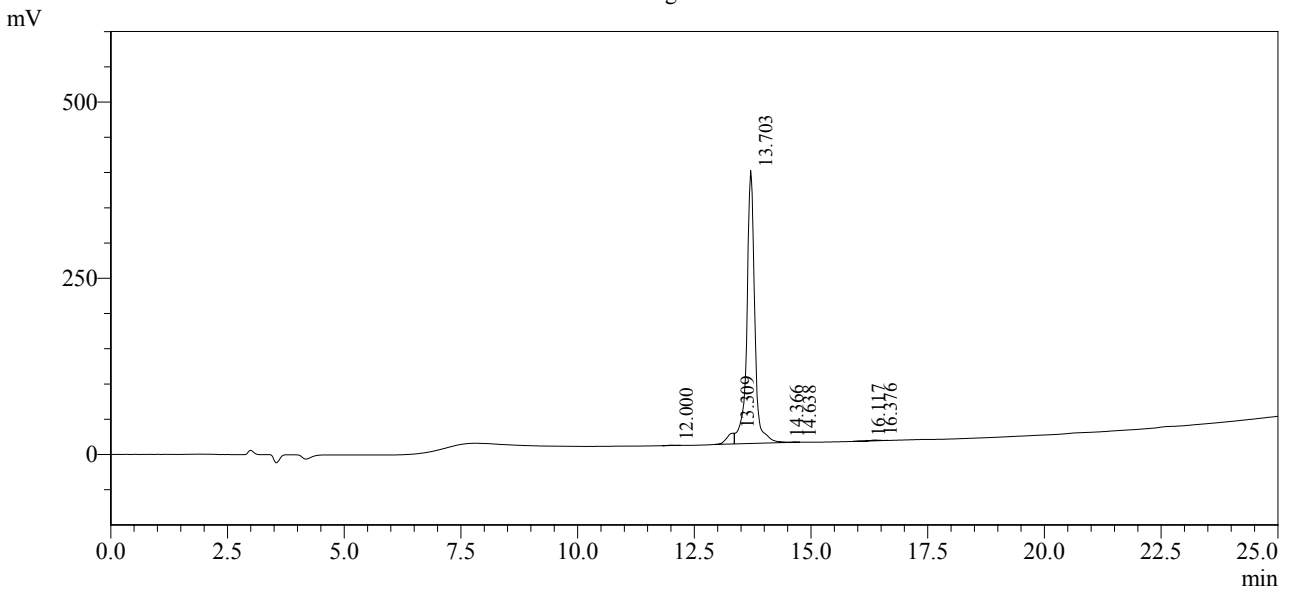

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.000	5670	590	0.119
2	13.309	171629	15295	3.602
3	13.703	4558194	387408	95.668
4	14.366	7594	1152	0.159
5	14.638	3455	365	0.073
6	16.117	2807	209	0.059
7	16.376	15247	925	0.320
Total		4764596	405944	100.000