


Mass Spectrum

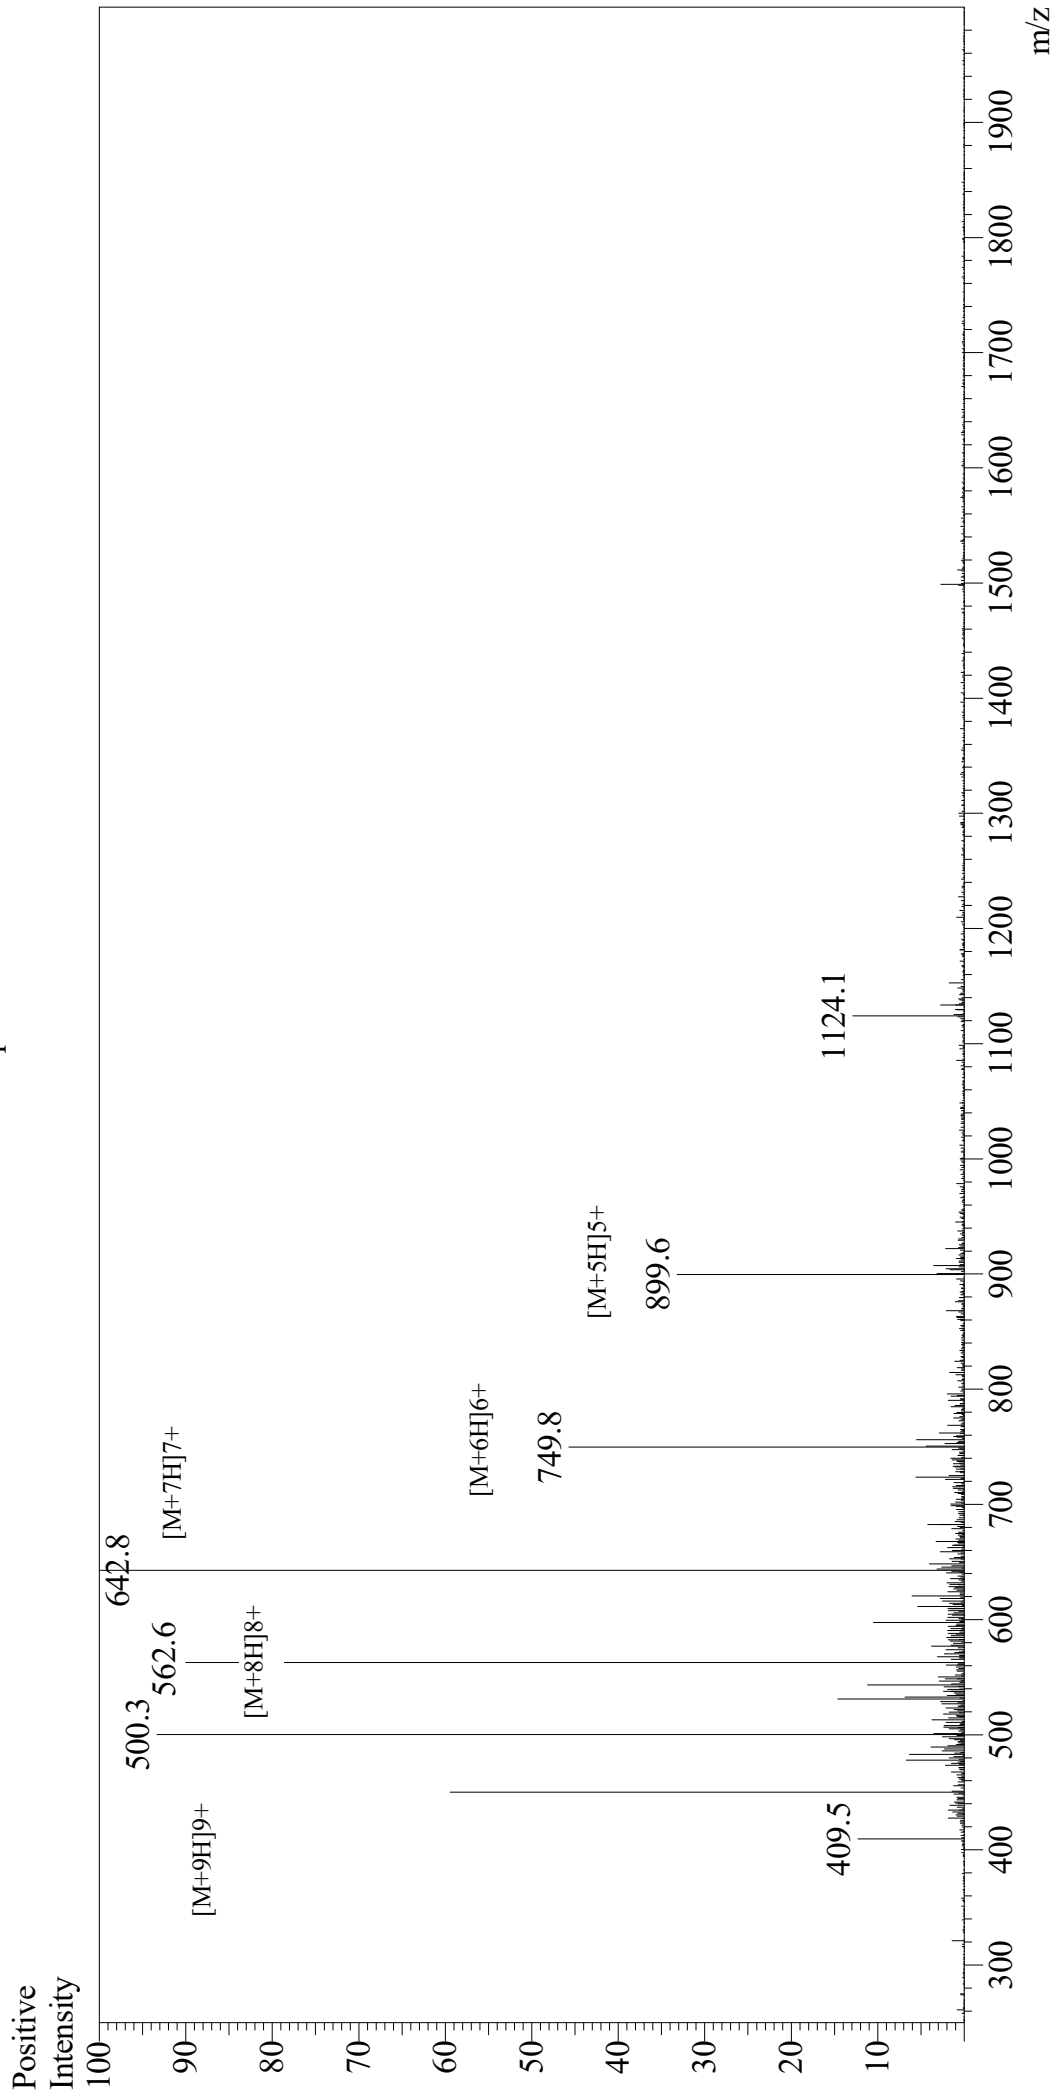

Sample Information

User : Gary
Month-Day Processed : 06/05/20
Time Processed : 03:23:13 PM
Injection Volume : 0.3
Sample Name : LL-37, scrambled
Cat No. : RP20332
Lot No. : E5114320F
Theoretical MW : 4493.30
Observed MW : 4492.7

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH