


Mass Spectrum

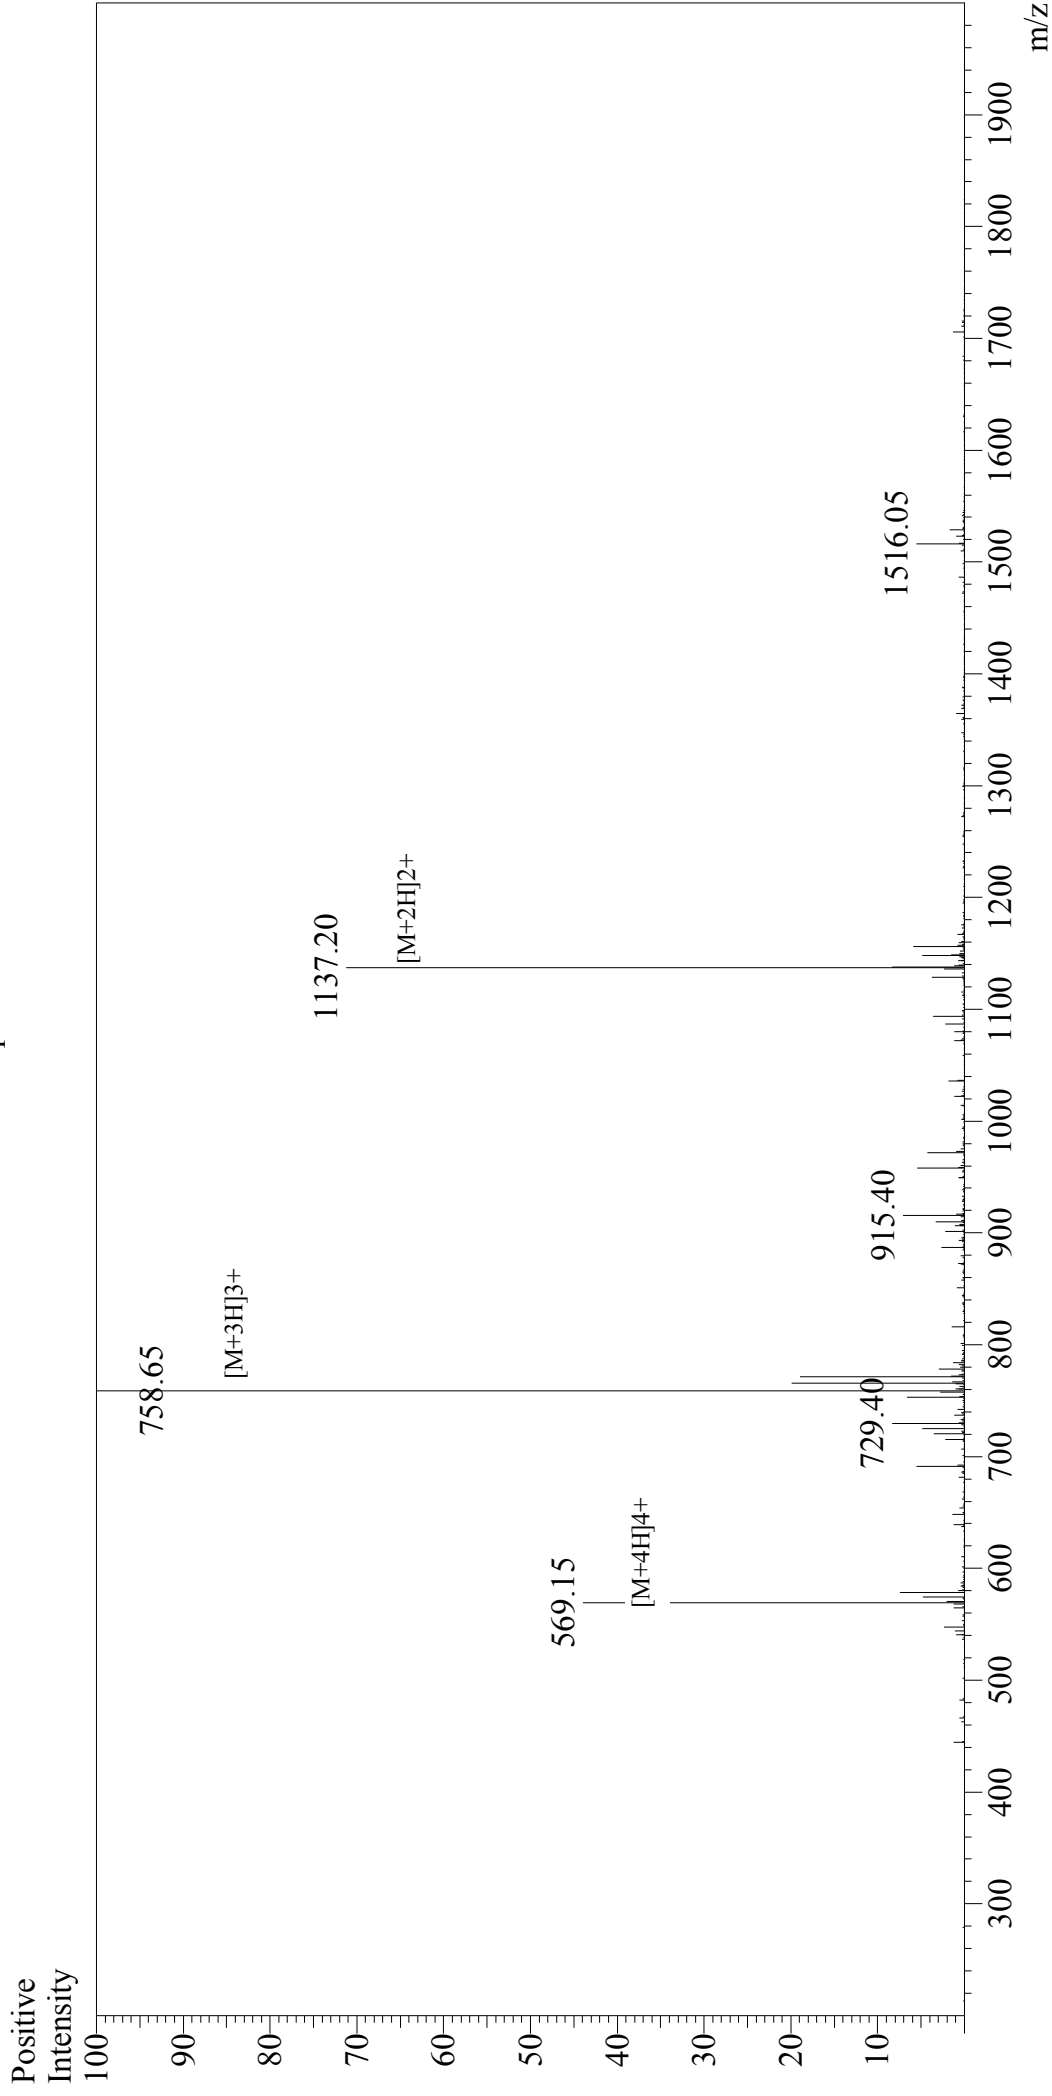

Sample Information

User : Gary
Month-Day Processed : 02/23/17
Time Processed : 12:47:49
Injection Volume : 0.2
Sample Name : Flagelin22
Cat No. : RPI9986
Lot No. : PE3081702
Theoretical MW : 2272.50
Observed MW : 2272.95

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH