

Sample Name : Hexa-His
 Cat. No.: RP11737
 Lot. No. : E5566819J
 Time Processed :7:27:40
 Month-Day-Year Processed :10/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

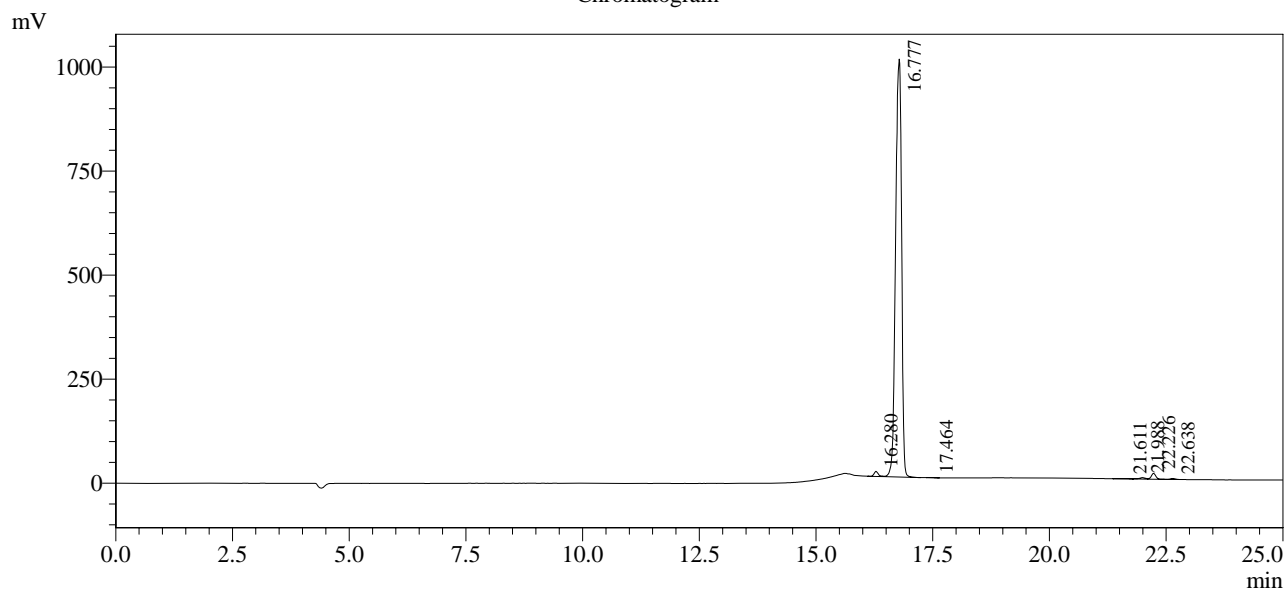

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.280	81606	12199	0.888
2	16.777	8955255	1004440	97.462
3	17.464	4239	688	0.046
4	21.611	4192	243	0.046
5	21.988	33276	3448	0.362
6	22.226	94238	14061	1.026
7	22.638	15658	2284	0.170
Total		9188463	1037362	100.000