

Sample Name:β-Amyloid (1-40)
 Cat No:RP10004
 Lot No :E7994320L
 Time Processed :5:16:22
 Month-Day-Year Processed :01/25/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

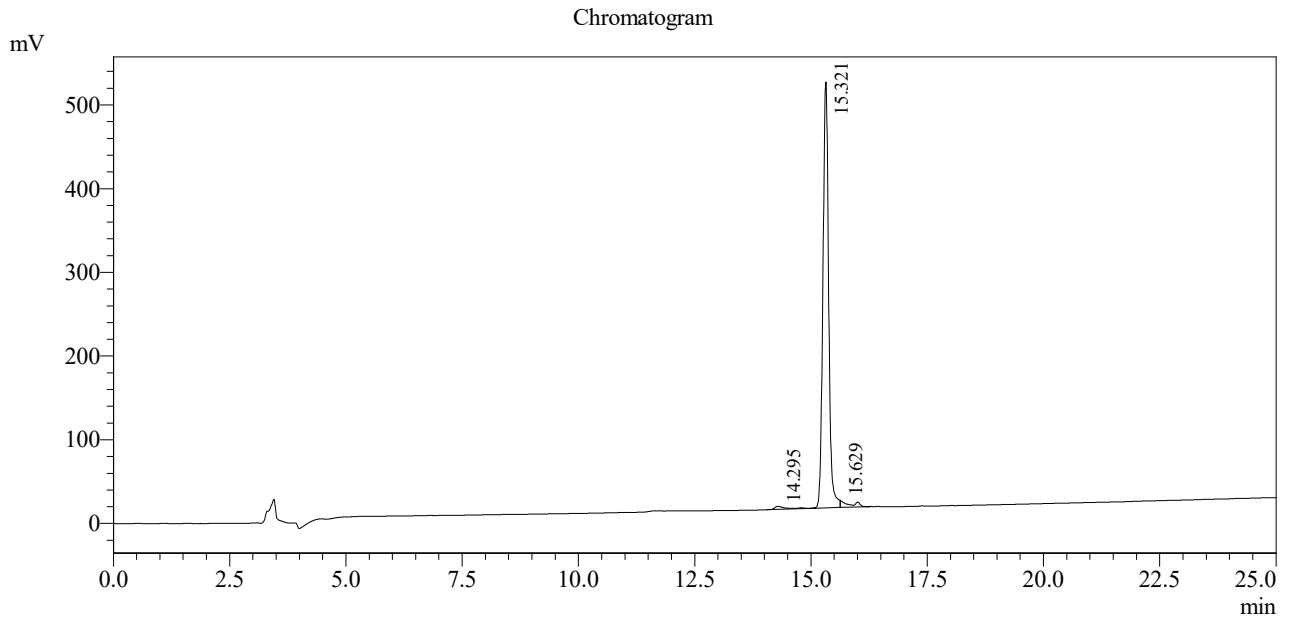

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.295	70347	3769	1.551
2	15.321	4348866	508997	95.872
3	15.629	116911	8550	2.577
Total		4536124	521316	100.000