

Sample Name : Hepatitis B Virus Core (128-140)
 Cat No.: RP17313
 Lot No.: E7253520B
 Time Processed : 9:51:45
 Month-Day-Year Processed : 02/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

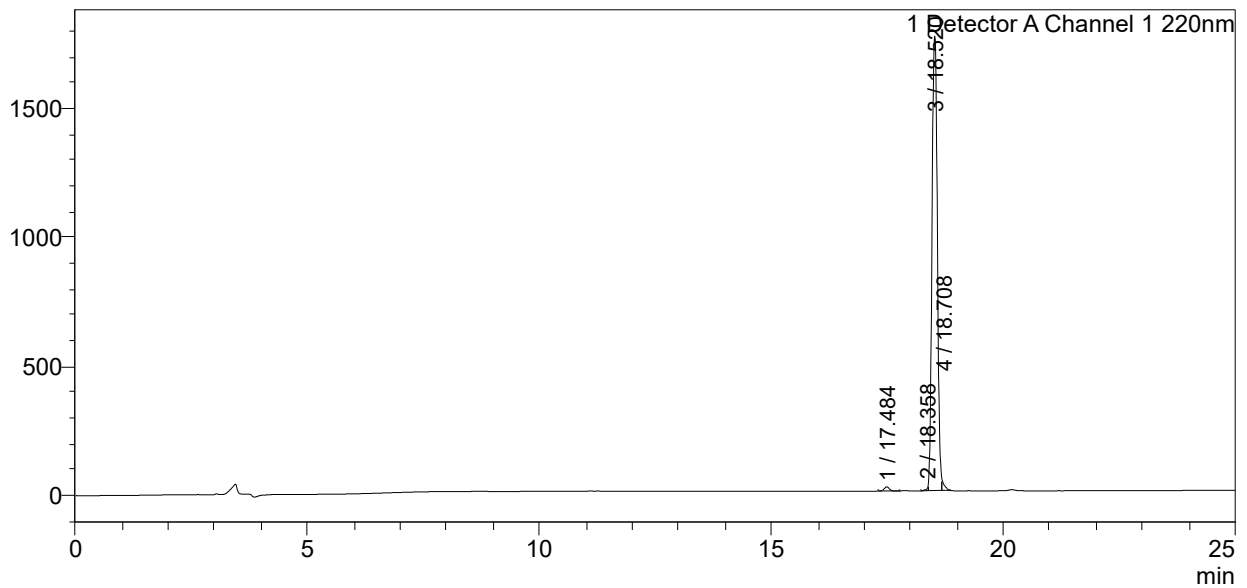

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.484	118932	15981	0.824
2	18.358	26740	6801	0.185
3	18.520	14194456	1763329	98.319
4	18.708	97001	26890	0.672
Total		14437129	1813000	100.000