


Sample Name : hgp100(25-33)
 Cat No : RP20344
 Lot NO : E7983820L
 Time Processed : 1:40:44 PM
 Month-Day-Year Processed : 12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
30.00	Pumps	B.Conc	95
35.00	Pumps	B.Conc	5
62.00	Pumps	B.Conc	5
70.00	Controller	Stop	

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

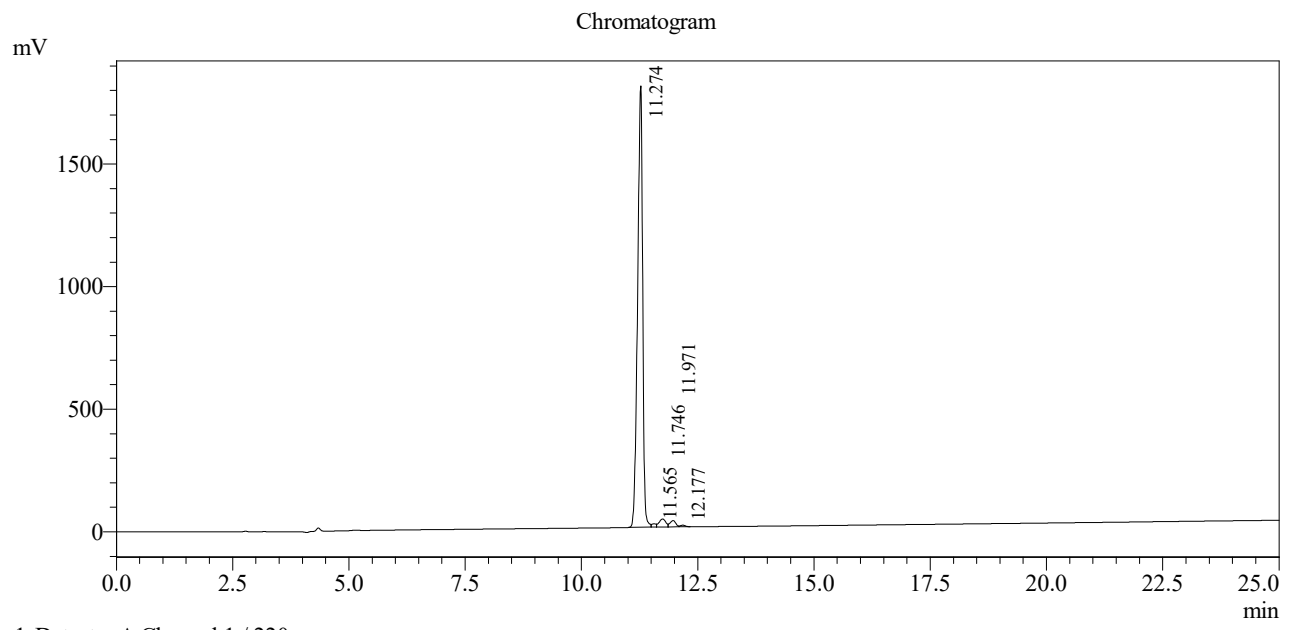

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.274	13550716	1800346	95.180
2	11.565	88005	13438	0.618
3	11.746	331912	32973	2.331
4	11.971	219533	25558	1.542
5	12.177	46788	6501	0.329
Total		14236954	1878816	100.000