

Sample Name :Neuropeptide Y, human
 Cat No. :RP10492
 Lot No. :E2875520B
 Time Processed :12:51:24
 Month-Day-Year Processed :02/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

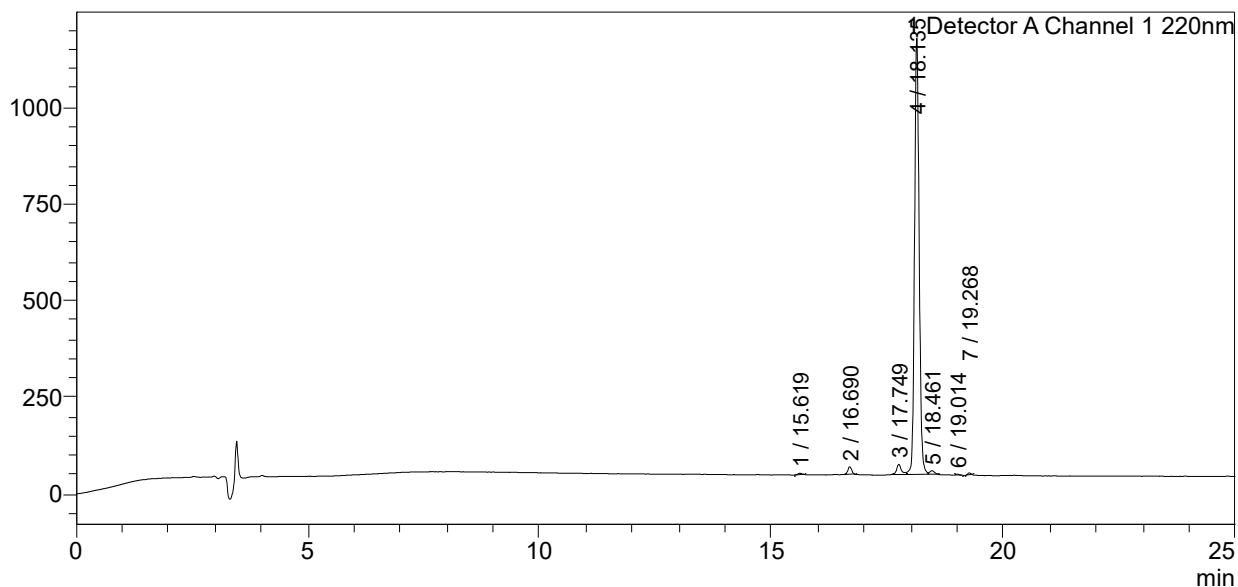

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.619	18612	3244	0.226
2	16.690	111660	19044	1.358
3	17.749	184000	25023	2.238
4	18.135	7820038	1052535	95.131
5	18.461	55536	8690	0.676
6	19.014	9761	2251	0.119
7	19.268	20647	4232	0.251
Total		8220253	1115019	100.000