

Sample Name : Amylin, human, amide  
 Cat. No. : RP11278  
 Lot. No. : E7942120H  
 Time Processed :13:11:43  
 Month-Day-Year Processed :09/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

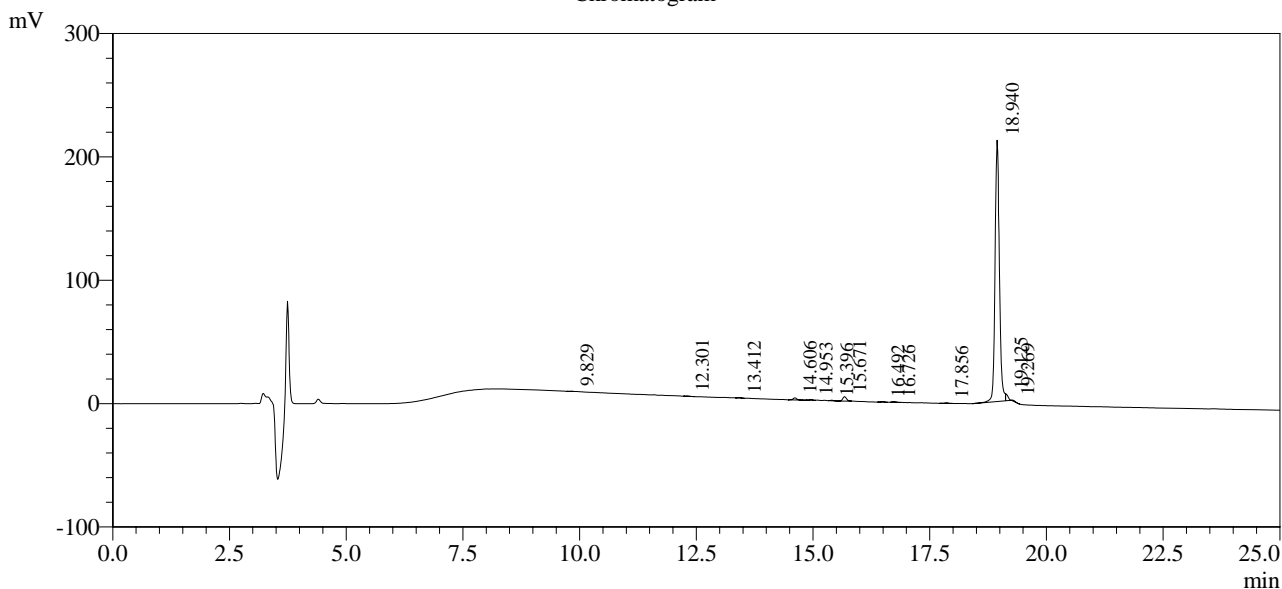

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.829	1018	196	0.071
2	12.301	1522	250	0.106
3	13.412	1982	385	0.138
4	14.606	9354	1701	0.651
5	14.953	2745	552	0.191
6	15.396	2286	459	0.159
7	15.671	19517	3584	1.359
8	16.492	2353	433	0.164
9	16.726	3209	575	0.223
10	17.856	3374	502	0.235
11	18.940	1368530	211769	95.283
12	19.125	17723	5640	1.234
13	19.269	2666	415	0.186
Total		1436279	226459	100.000